
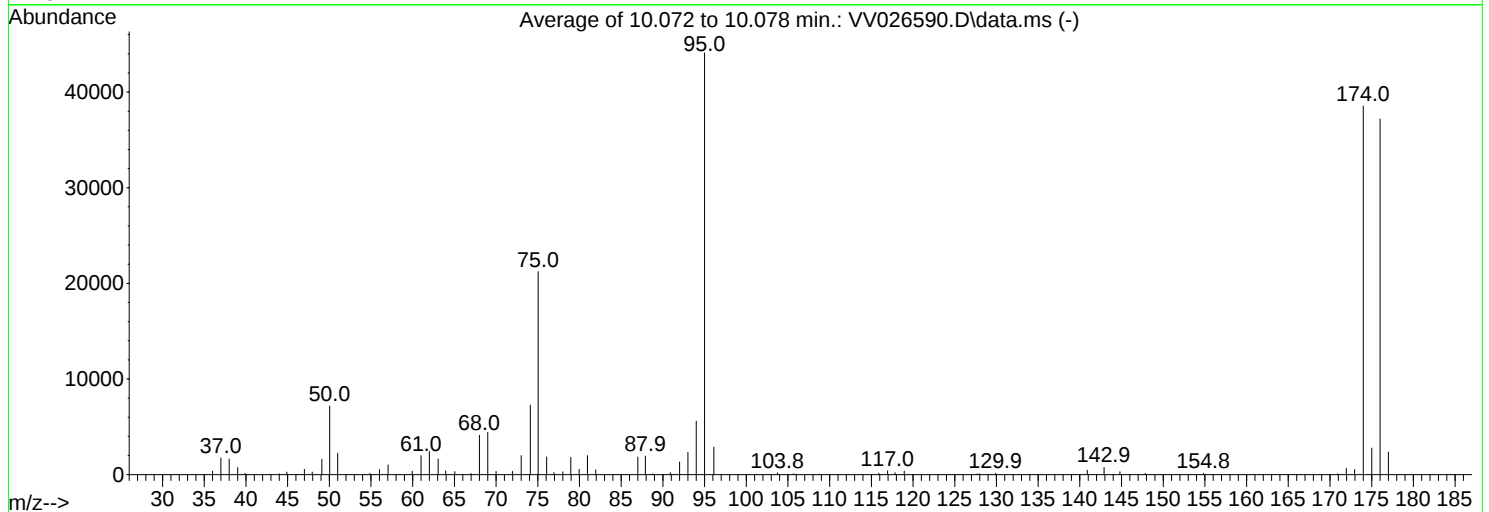


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062922\
 Data File : VV026590.D
 Acq On : 29 Jun 2022 15:17
 Operator : SY/MD
 Sample : BFB292
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB292

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis
 Last Update : Fri Jul 01 00:19:36 2022

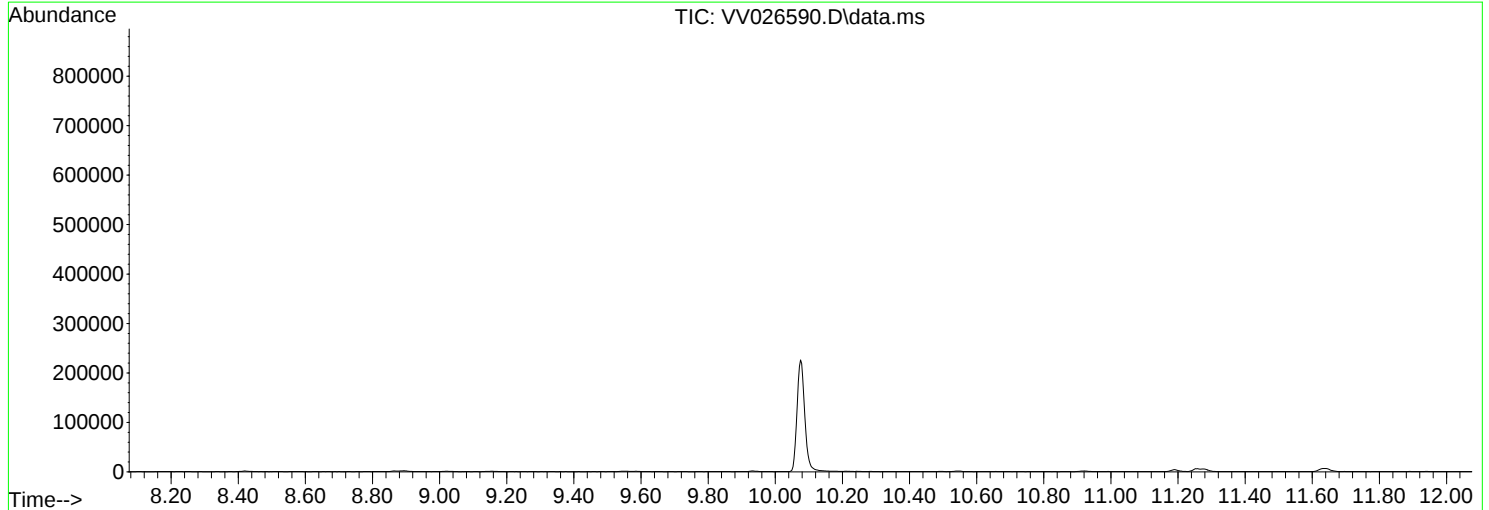

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	7185	PASS
75	95	30	80	48.2	21237	PASS
95	95	100	100	100.0	44104	PASS
96	95	5	9	6.5	2874	PASS
173	174	0.00	2	1.4	544	PASS
174	95	50	120	87.4	38547	PASS
175	174	5	9	7.2	2779	PASS
176	174	95	105	96.5	37184	PASS
177	176	5	10	6.3	2353	PASS

m/z	Abundance
39.90	123.0
44.00	585.0

Instrument :
MSVOA_V
ClientSampleId :
BFB292

m/z	Abundance
36.00	411.0
37.00	1756.0
38.00	1630.0
39.00	758.0
39.90	236.0
44.00	636.0
44.90	289.0
46.10	104.0
47.00	548.0
48.00	261.0
49.10	1616.0
50.00	7315.0
51.00	2147.0
52.10	101.0
54.90	113.0
56.00	548.0
57.00	1042.0
60.00	342.0
61.00	1902.0
62.00	2542.0
63.10	1552.0
64.00	402.0
65.00	347.0
66.90	120.0
68.00	4043.0
69.00	4218.0
70.00	265.0
71.90	303.0
73.00	1847.0
74.10	7027.0
75.10	20904.0
76.10	1903.0
76.90	232.0
78.00	265.0
78.90	1774.0
79.90	529.0
81.00	1927.0
82.00	474.0
87.10	1717.0
87.90	1808.0
90.90	237.0
92.00	1315.0
93.00	2143.0
94.00	5531.0
95.00	43520.0
96.10	2986.0
103.80	170.0
106.00	147.0
115.90	120.0
117.00	374.0
117.80	158.0
118.90	346.0
127.70	190.0
129.90	141.0
140.90	449.0
142.90	682.0
144.80	264.0
147.90	144.0
154.80	121.0
170.90	123.0
171.90	569.0
172.90	472.0
174.00	36416.0
175.00	2660.0
176.00	35640.0
177.00	2293.0

Instrument :
MSVOA_V
ClientSampleId :
BFB292

m/z	Abundance
36.00	378.0
37.00	1820.0
38.00	1634.0
39.00	769.0
39.90	258.0
44.00	682.0
44.90	283.0
47.00	567.0
47.90	282.0
49.10	1710.0
50.00	7373.0
51.00	2313.0
54.80	113.0
56.00	563.0
57.10	1042.0
59.90	375.0
61.00	2009.0
62.00	2528.0
63.00	1691.0
64.00	400.0
65.10	304.0
67.00	120.0
68.00	4291.0
69.00	4513.0
70.00	353.0
72.00	380.0
73.00	2091.0
74.10	7573.0
75.00	21984.0
76.10	1873.0
76.90	206.0
78.00	303.0
79.00	1864.0
79.90	575.0
81.00	2080.0
82.00	519.0
87.00	1903.0
87.90	2031.0
88.80	128.0
90.90	206.0
92.00	1376.0
93.00	2385.0
94.00	5783.0
95.00	45520.0
96.10	2912.0
103.70	198.0
105.70	136.0
115.90	172.0
116.90	413.0
117.90	216.0
118.90	378.0
128.00	159.0
129.90	152.0
140.90	482.0
142.90	769.0
144.80	317.0
145.90	104.0
147.80	136.0
153.80	110.0
154.80	140.0
170.90	104.0
172.00	677.0
172.90	560.0
174.00	39552.0
175.00	2879.0
176.00	38408.0
177.00	2403.0

Instrument :
MSVOA_V
ClientSampleId :
BFB292

m/z	Abundance
36.00	312.0
37.00	1649.0
38.00	1587.0
39.00	698.0
39.90	273.0
44.00	677.0
44.90	253.0
47.00	546.0
47.90	275.0
49.10	1506.0
50.10	6866.0
51.00	2248.0
54.90	108.0
56.00	494.0
57.10	1000.0
59.90	379.0
61.00	2041.0
62.00	2211.0
63.10	1684.0
63.90	361.0
65.10	295.0
67.10	110.0
68.00	4040.0
69.00	4518.0
70.00	409.0
72.00	376.0
73.00	2023.0
74.10	7259.0
75.00	20824.0
76.00	1750.0
77.00	200.0
78.00	317.0
78.90	1801.0
80.00	553.0
80.90	1964.0
81.90	498.0
86.90	1922.0
87.90	2000.0
88.80	119.0
90.90	169.0
92.00	1276.0
93.00	2425.0
94.00	5467.0
95.00	43272.0
96.10	2725.0
103.70	205.0
105.70	133.0
115.90	178.0
116.90	396.0
117.90	221.0
119.00	361.0
127.90	155.0
129.90	175.0
140.90	478.0
142.90	822.0
144.80	333.0
147.80	123.0
154.90	144.0
156.90	107.0
172.00	721.0
173.00	599.0
174.00	39672.0
175.00	2797.0
176.00	37504.0
177.00	2363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB292