

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070124\
 Data File : VV036405.D
 Acq On : 02 Jul 2024 03:42
 Operator : SY/MD
 Sample : P3087-24
 Misc : 4.77g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 02 05:29:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 02 05:19:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	592309	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	564099	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	229102	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	138658	13.784	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.120%
7) Chloroethane-d5	1.526	69	130763	16.275	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.080%
11) 1,1-Dichloroethene-d2	2.050	65	65590	13.870	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.480%
21) 2-Butanone-d5	3.857	46	9711	4.160	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	8.320%#
24) Chloroform-d	4.240	84	312440	17.870	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.480%
26) 1,2-Dichloroethane-d4	4.937	65	166394	17.846	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	71.400%
32) Benzene-d6	4.953	84	572934	17.992	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.960%
36) 1,2-Dichloropropane-d6	5.982	67	188951	19.727	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	78.920%
41) Toluene-d8	7.239	98	475727	16.570	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	66.280%
43) trans-1,3-Dichloroprop...	7.551	79	55841	13.055	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	52.240%
47) 2-Hexanone-d5	8.034	63	17449	11.413	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	22.820%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	132063	16.820	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	67.280%
66) 1,2-Dichlorobenzene-d4	11.558	152	163444	19.577	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.320%
Target Compounds						
					Qvalue	
35) Methylcyclohexane	5.985	83	46872	3.190	ug/L	# 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070124\
Data File : VV036405.D
Acq On : 02 Jul 2024 03:42
Operator : SY/MD
Sample : P3087-24
Misc : 4.77g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jul 02 05:29:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 02 05:19:46 2024
Response via : Initial Calibration

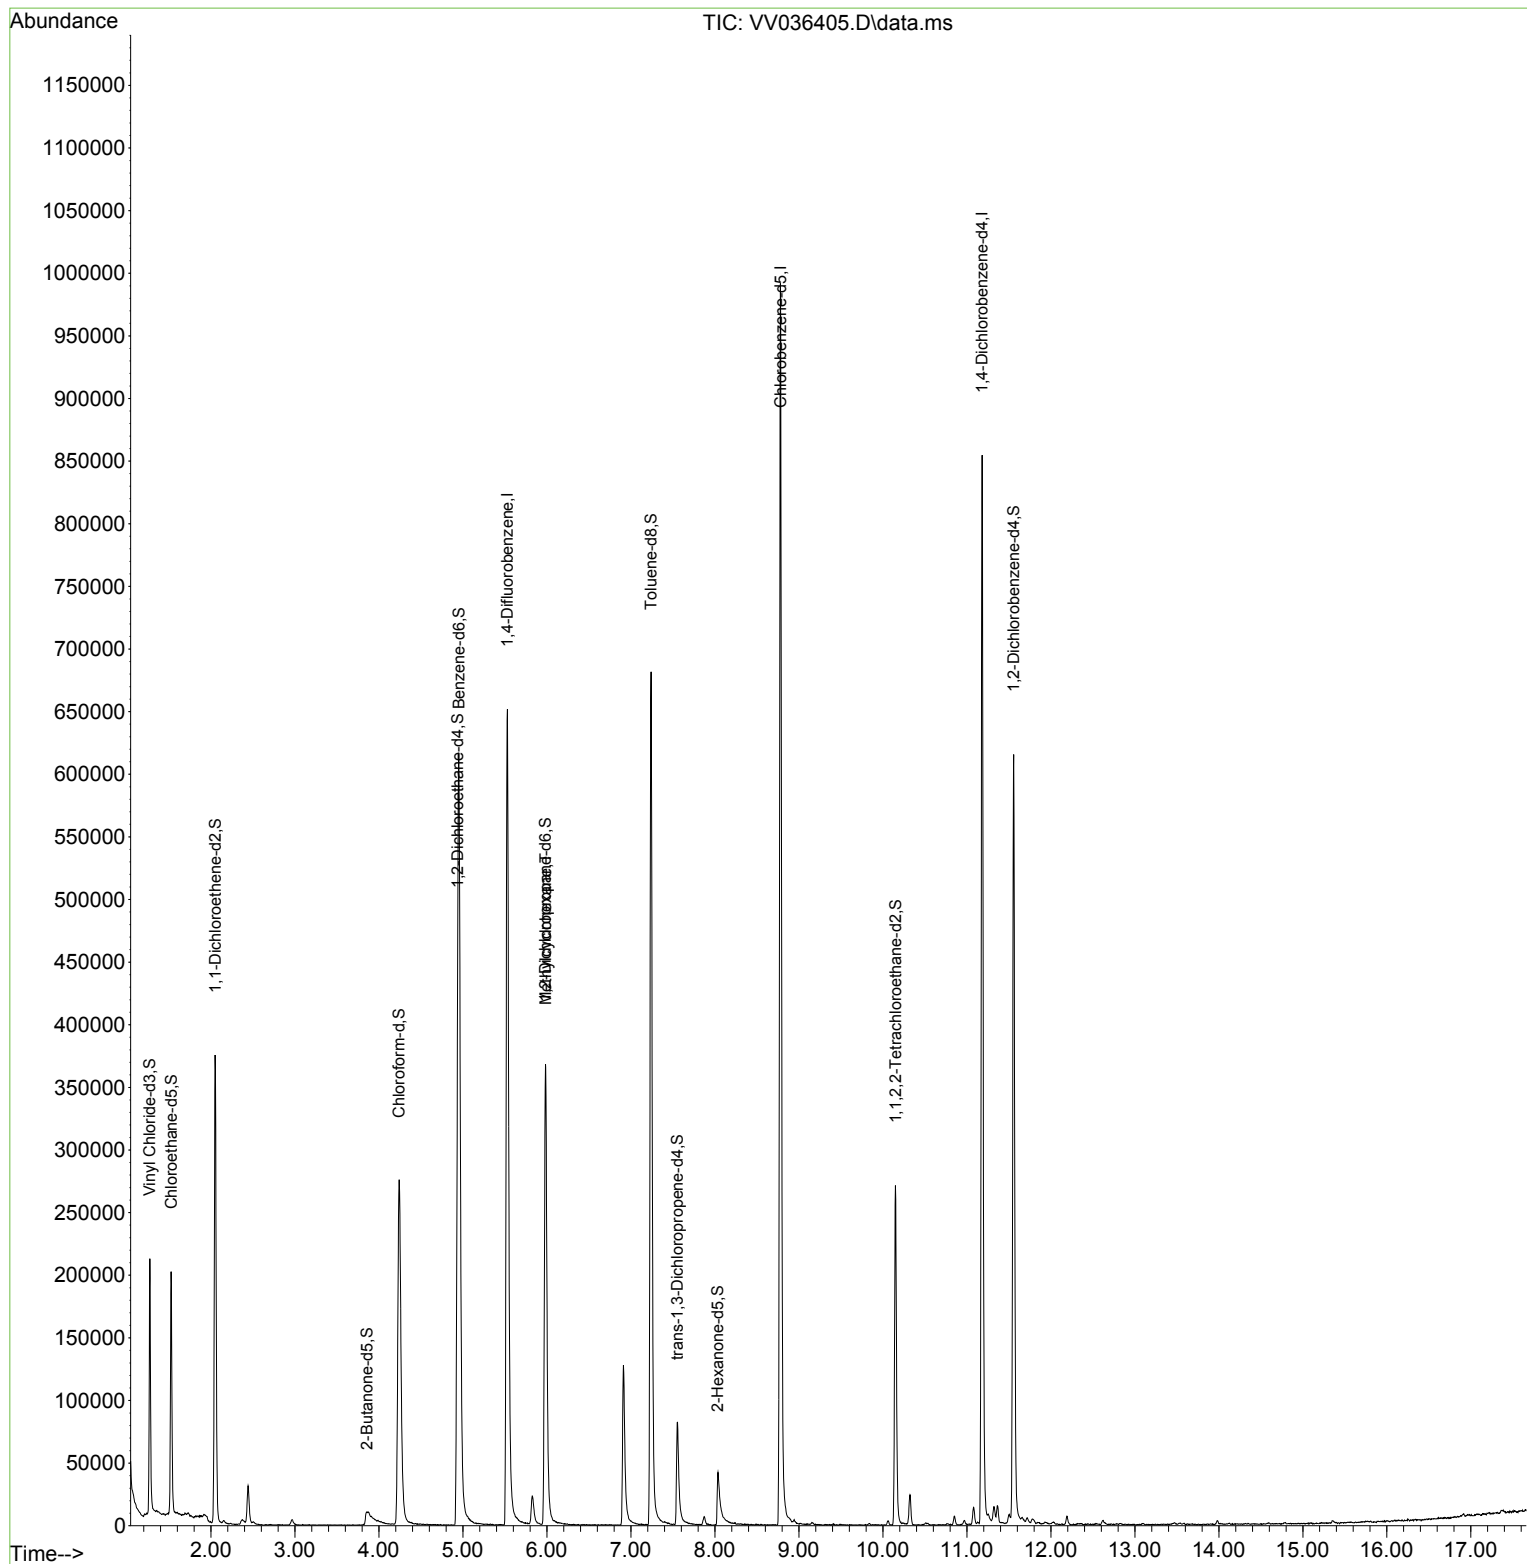

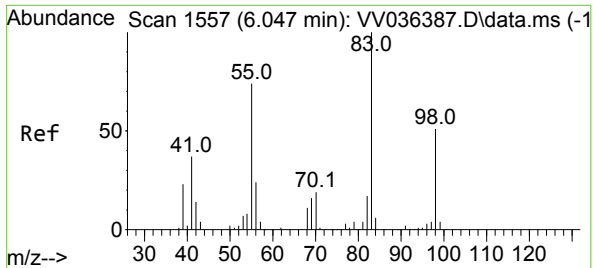

#35
Methylcyclohexane
Concen: 3.190 ug/L
RT: 5.985 min Scan# 11
Delta R.T. -0.061 min
Lab File: VV036405.D
Acq: 02 Jul 2024 03:42

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 83 Resp: 46872
Ion Ratio Lower Upper
83 100
55 0.5 56.0 84.0#
98 1.6 39.0 58.6#

