

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW070124\
 Data File : VW036377.D
 Acq On : 01 Jul 2024 15:48
 Operator : SY/MD
 Sample : VIBLK310
 Misc : 5.00g/10.0mL/MSVOA_V/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK310

Quant Time: Jul 02 02:39:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 02 02:29:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	321916	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	339425	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	144561	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	123521	22.593	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.360%
7) Chloroethane-d5	1.526	69	105489	24.157	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.640%
11) 1,1-Dichloroethene-d2	2.050	65	58230	22.657	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	90.640%
21) 2-Butanone-d5	3.838	46	43519	34.298	ug/L	-0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.600%
24) Chloroform-d	4.243	84	220534	23.209	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.840%
26) 1,2-Dichloroethane-d4	4.937	65	122868	24.247	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.000%
32) Benzene-d6	4.953	84	410963	21.448	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.800%
36) 1,2-Dichloropropane-d6	5.985	67	134997	23.423	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.680%
41) Toluene-d8	7.239	98	339333	19.642	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.560%
43) trans-1,3-Dichloroprop...	7.555	79	51954	20.187	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.760%
47) 2-Hexanone-d5	8.030	63	33592	36.514	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.020%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	113476	24.020	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.080%
66) 1,2-Dichlorobenzene-d4	11.558	152	130057	24.688	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.760%
Target Compounds						
67) 1,2-Dichlorobenzene	11.574	146	9920	1.141	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070124\
Data File : VV036377.D
Acq On : 01 Jul 2024 15:48
Operator : SY/MD
Sample : VIBLK310
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK310

Quant Time: Jul 02 02:39:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 02 02:29:42 2024
Response via : Initial Calibration

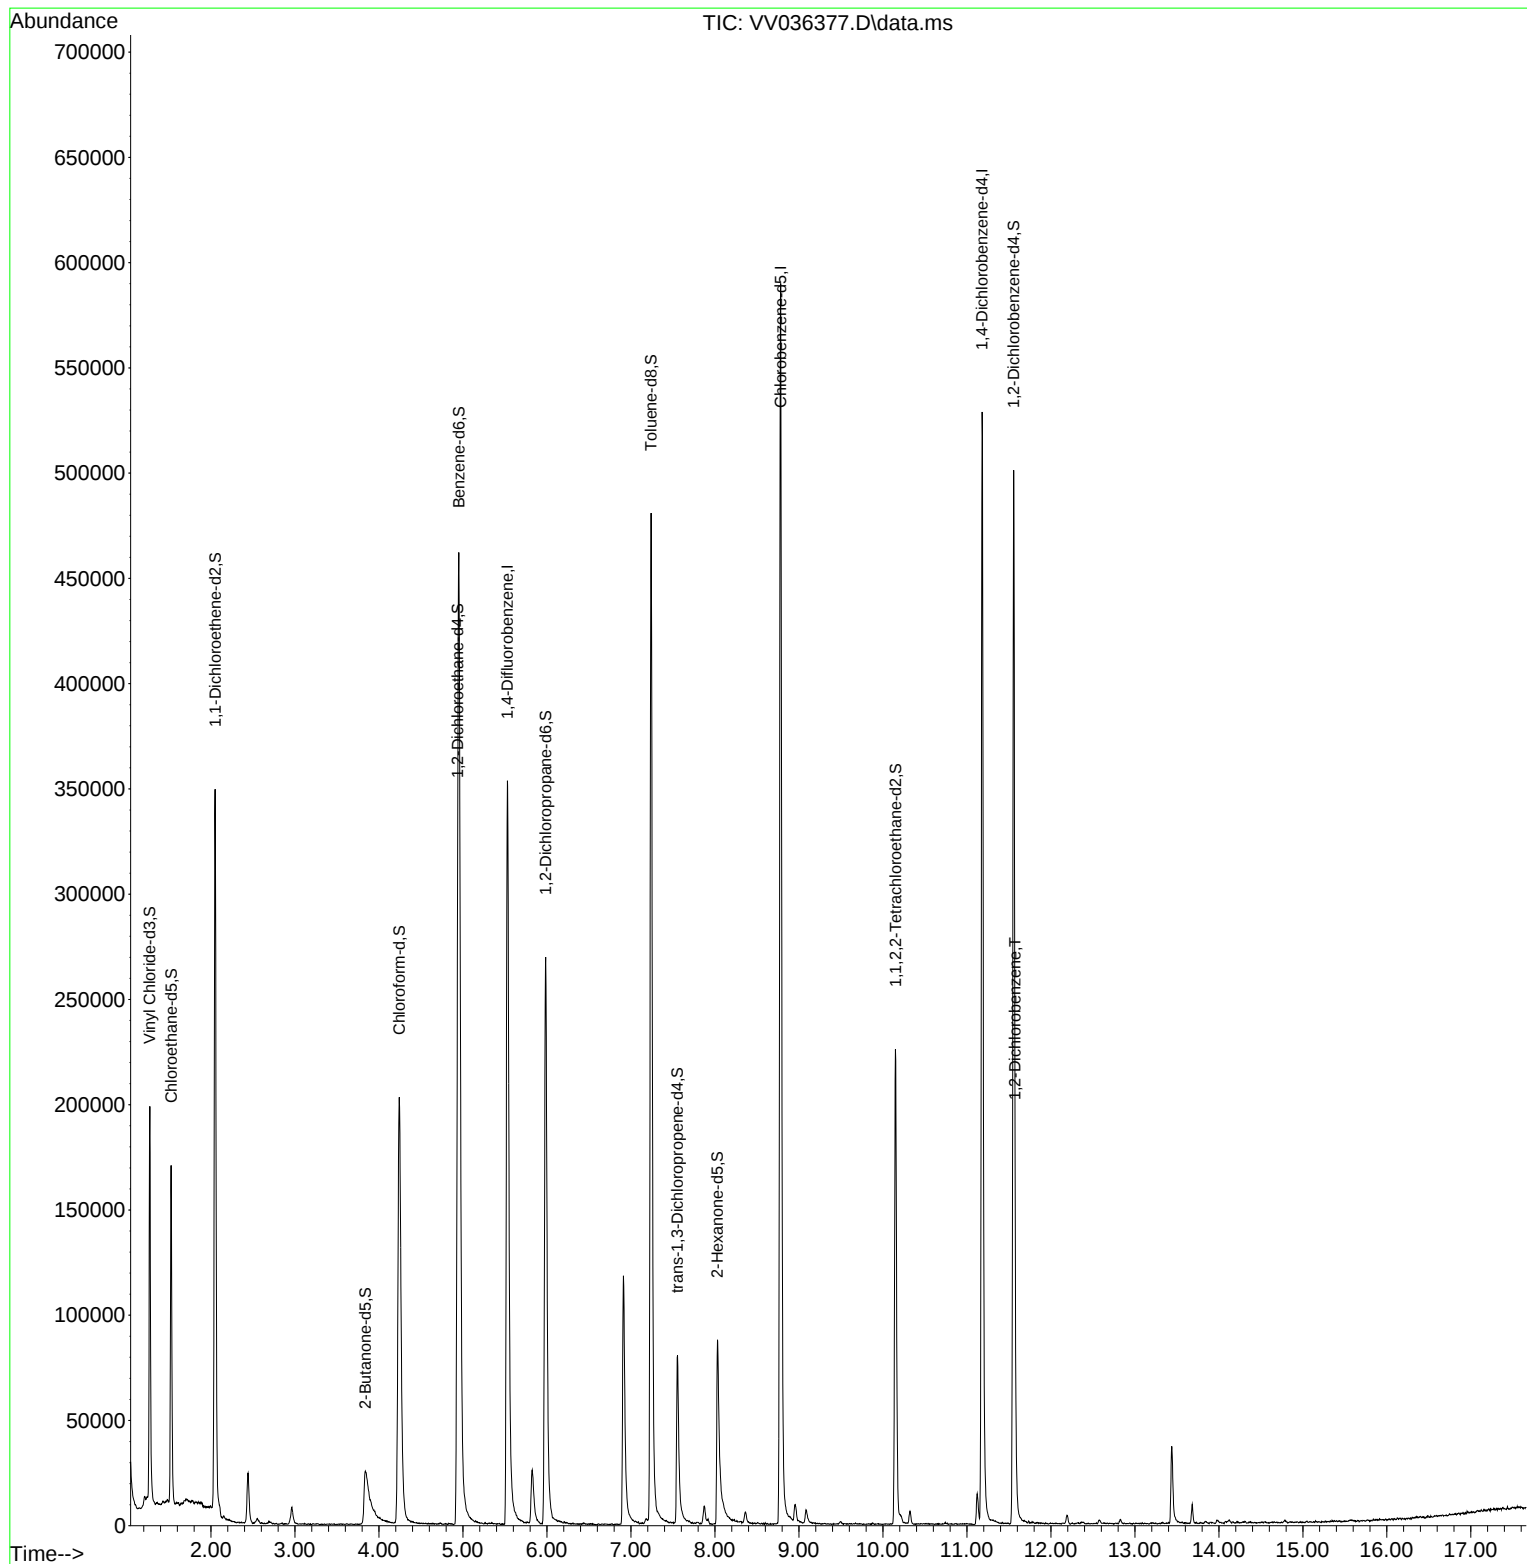

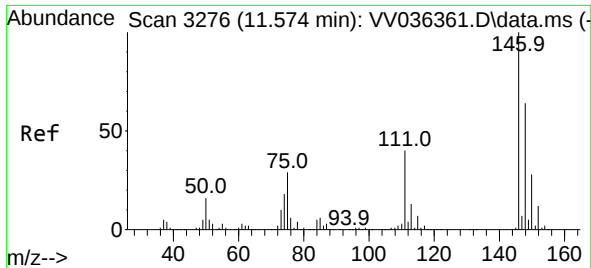

#67
 1,2-Dichlorobenzene
 Concen: 1.141 ug/L
 RT: 11.574 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VV036377.D
 Acq: 01 Jul 2024 15:48

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK310

Tgt Ion:146 Resp: 9920
 Ion Ratio Lower Upper
 146 100
 111 48.4 33.3 49.9
 148 67.8 51.1 76.7

