
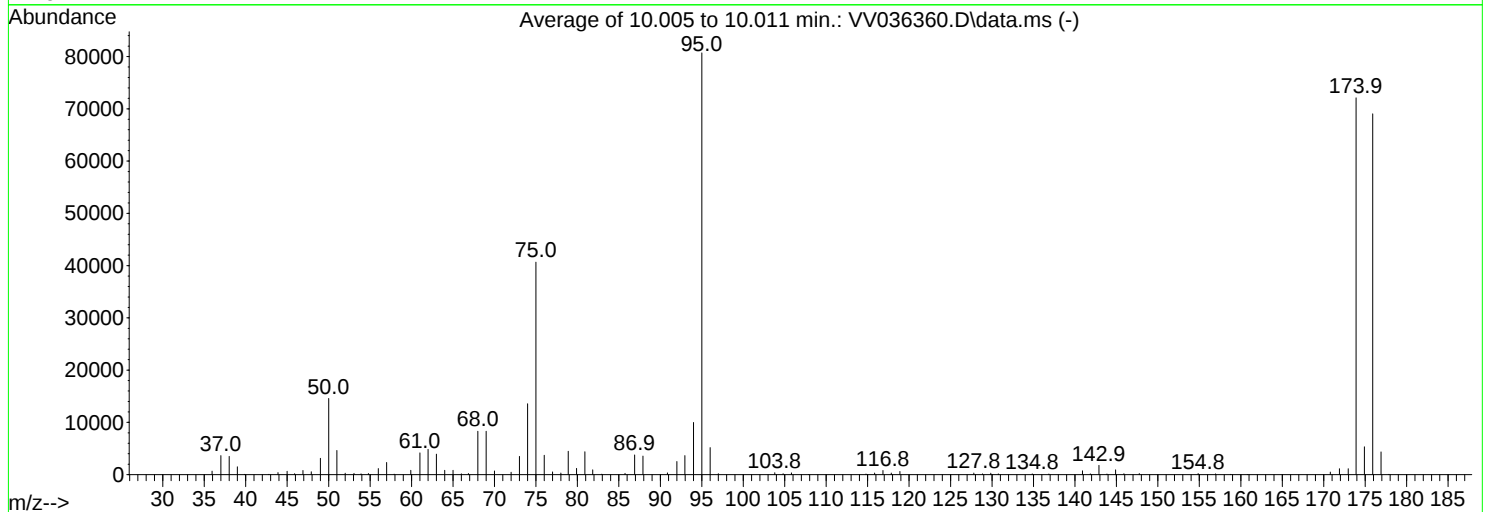


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070124\
Data File : VV036360.D
Acq On : 01 Jul 2024 08:59
Operator : SY/MD
Sample : BFB333
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB333

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Title : VOC Analysis
Last Update : Thu Jul 04 02:05:51 2024

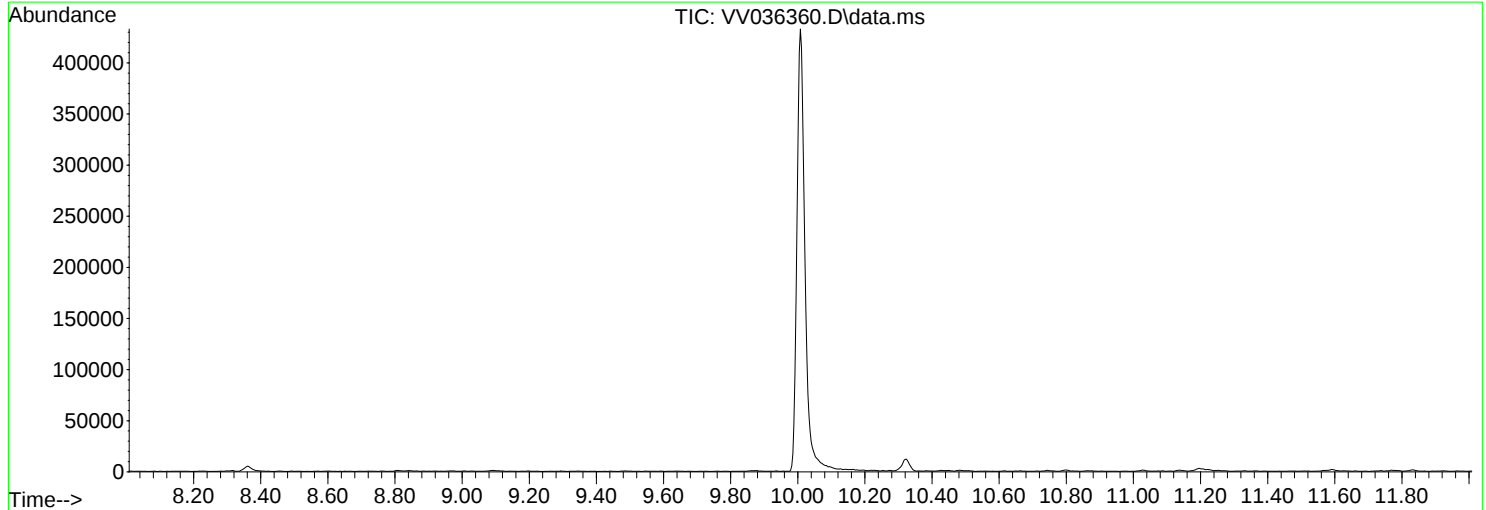

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	14585	PASS
75	95	30	80	50.4	40664	PASS
95	95	100	100	100.0	80715	PASS
96	95	5	9	6.4	5190	PASS
173	174	0.00	2	1.6	1149	PASS
174	95	50	120	89.3	72093	PASS
175	174	5	9	7.4	5335	PASS
176	174	95	101	95.8	69037	PASS
177	176	5	9	6.3	4355	PASS

m/z	Abundance
39.80	212.0
44.00	464.0

Instrument :
MSVOA_V
ClientSampleId :
BFB333

m/z	Abundance
36.00	649.0
37.00	3623.0
38.00	3393.0
39.00	1441.0
40.00	291.0
42.80	102.0
43.90	909.0
45.00	670.0
45.90	229.0
46.90	728.0
47.90	533.0
49.00	3031.0
50.00	14617.0
51.00	4516.0
52.00	306.0
53.10	247.0
53.90	148.0
54.80	209.0
56.00	1072.0
57.00	2310.0
57.90	120.0
59.90	864.0
61.00	4057.0
62.00	4819.0
63.00	3861.0
64.00	852.0
65.00	755.0
65.90	178.0
66.80	221.0
68.00	7991.0
69.00	8106.0
70.00	674.0
72.00	450.0
73.00	3408.0
74.00	13111.0
75.00	40200.0
76.00	3859.0
77.00	549.0
78.00	311.0
78.90	4527.0
79.90	1111.0
80.90	4312.0
81.80	894.0
85.70	202.0
86.90	3853.0
87.90	3529.0
90.90	302.0
92.00	2450.0
93.00	3549.0
94.00	9725.0
95.00	79832.0
96.00	5181.0
97.00	202.0
103.80	341.0
104.80	177.0
105.80	309.0
114.80	131.0
115.80	354.0
116.80	769.0
117.90	278.0
118.90	610.0
127.70	291.0
129.00	151.0
129.90	233.0
130.70	164.0
134.80	133.0
136.80	134.0
140.90	722.0
141.80	133.0
142.90	1689.0
143.90	129.0
144.90	945.0
145.90	193.0
147.80	188.0
154.90	242.0
156.90	143.0
170.80	472.0
171.90	1021.0
172.90	1130.0
173.90	69176.0
174.90	5206.0
175.90	66792.0
176.90	4441.0
177.90	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB333

m/z	Abundance
36.00	673.0
37.00	3761.0
38.00	3576.0
39.00	1559.0
39.90	268.0
42.80	102.0
43.90	907.0
45.00	664.0
45.90	198.0
46.90	819.0
47.90	566.0
49.00	3229.0
50.00	15105.0
51.00	4749.0
52.00	295.0
53.10	261.0
53.90	156.0
54.80	219.0
56.00	1187.0
57.00	2444.0
57.90	108.0
59.90	866.0
61.00	4292.0
62.00	5056.0
63.00	4061.0
64.00	858.0
65.00	841.0
66.00	147.0
66.80	206.0
68.00	8610.0
69.00	8548.0
70.00	725.0
72.00	473.0
73.00	3592.0
74.00	13983.0
75.00	42136.0
76.00	3859.0
77.00	525.0
78.00	319.0
78.90	4660.0
79.90	1233.0
80.90	4549.0
81.80	949.0
83.00	101.0
85.80	248.0
86.90	3905.0
87.90	3694.0
90.80	351.0
92.00	2605.0
92.90	3784.0
94.00	10306.0
95.00	83568.0
96.00	5355.0
97.00	205.0
103.80	370.0
104.80	183.0
105.80	339.0
114.80	123.0
115.80	340.0
116.80	809.0
117.80	316.0
118.90	661.0
127.80	321.0
128.80	164.0
129.80	288.0
130.80	150.0
134.80	153.0
136.90	120.0
140.90	752.0
141.90	164.0
142.90	1826.0
143.80	106.0
144.90	961.0
145.90	194.0
147.70	231.0
154.90	230.0
157.00	141.0
158.80	108.0
160.80	104.0
170.80	523.0
171.90	1155.0
172.90	1164.0
173.90	74424.0
174.90	5537.0
175.90	71232.0
176.90	4505.0

Instrument :
MSVOA_V
ClientSampleId :
BFB333

m/z	Abundance
35.90	673.0
37.00	3511.0
38.00	3508.0
39.00	1536.0
39.80	257.0
43.90	798.0
45.00	572.0
45.90	157.0
46.90	858.0
47.90	533.0
49.00	3099.0
50.00	14033.0
51.00	4616.0
52.00	271.0
53.00	269.0
53.90	136.0
54.80	205.0
56.00	1203.0
57.00	2267.0
57.90	104.0
59.90	787.0
61.00	4135.0
62.00	4667.0
63.00	3819.0
64.00	777.0
65.00	870.0
66.10	105.0
66.90	195.0
68.00	8265.0
69.00	8206.0
70.00	732.0
72.00	458.0
73.00	3470.0
74.00	13643.0
75.00	39656.0
76.00	3366.0
77.00	513.0
78.00	303.0
78.90	4265.0
79.90	1220.0
80.90	4321.0
81.90	924.0
82.90	143.0
85.80	260.0
86.90	3537.0
87.90	3477.0
90.80	365.0
92.00	2469.0
92.90	3565.0
94.00	9927.0
95.00	78744.0
96.00	5033.0
97.00	158.0
103.80	357.0
104.80	162.0
105.80	355.0
107.90	137.0
114.80	115.0
115.90	273.0
116.90	806.0
117.80	368.0
118.90	617.0
127.90	316.0
128.80	166.0
129.80	334.0
130.80	114.0
134.90	142.0
136.90	117.0
140.90	740.0
141.90	151.0
142.90	1776.0
143.80	100.0
144.90	870.0
145.90	156.0
147.70	229.0
154.80	202.0
156.90	154.0
158.80	107.0
161.00	107.0
170.80	496.0
171.90	1244.0
173.00	1152.0
173.90	72680.0
174.90	5263.0
175.90	69088.0
176.90	4119.0
177.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB333