

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW070224\
 Data File : VW036417.D
 Acq On : 02 Jul 2024 13:28
 Operator : SY/MD
 Sample : P3087-15
 Misc : 5.82g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 03 05:11:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 03 05:08:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	544894	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	448330	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	123467	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	162144	17.522	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.080%
7) Chloroethane-d5	1.526	69	132046	17.865	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.440%
11) 1,1-Dichloroethene-d2	2.050	65	71789	16.502	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.000%
21) 2-Butanone-d5	3.851	46	21455	9.990	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	19.980%#
24) Chloroform-d	4.243	84	265838	16.528	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	66.120%
26) 1,2-Dichloroethane-d4	4.937	65	136622	15.928	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	63.720%#
32) Benzene-d6	4.953	84	522424	20.642	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.560%
36) 1,2-Dichloropropane-d6	5.986	67	156722	20.587	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.360%
41) Toluene-d8	7.240	98	411877	18.050	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.200%
43) trans-1,3-Dichloroprop...	7.551	79	52536	15.454	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	61.800%
47) 2-Hexanone-d5	8.034	63	28020	23.059	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	46.120%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	91249	14.623	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	58.480%
66) 1,2-Dichlorobenzene-d4	11.558	152	78181	17.376	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	69.520%#
Target Compounds						
					Qvalue	
13) Acetone	2.143	43	4935	1.701	ug/L #	1
14) Carbon disulfide	2.233	76	17640	0.651	ug/L	98
35) Methylcyclohexane	5.986	83	38737	3.317	ug/L #	22
48) 2-Hexanone	8.037	43	3229	1.073	ug/L #	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070224\
Data File : VV036417.D
Acq On : 02 Jul 2024 13:28
Operator : SY/MD
Sample : P3087-15
Misc : 5.82g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jul 03 05:11:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 03 05:08:41 2024
Response via : Initial Calibration

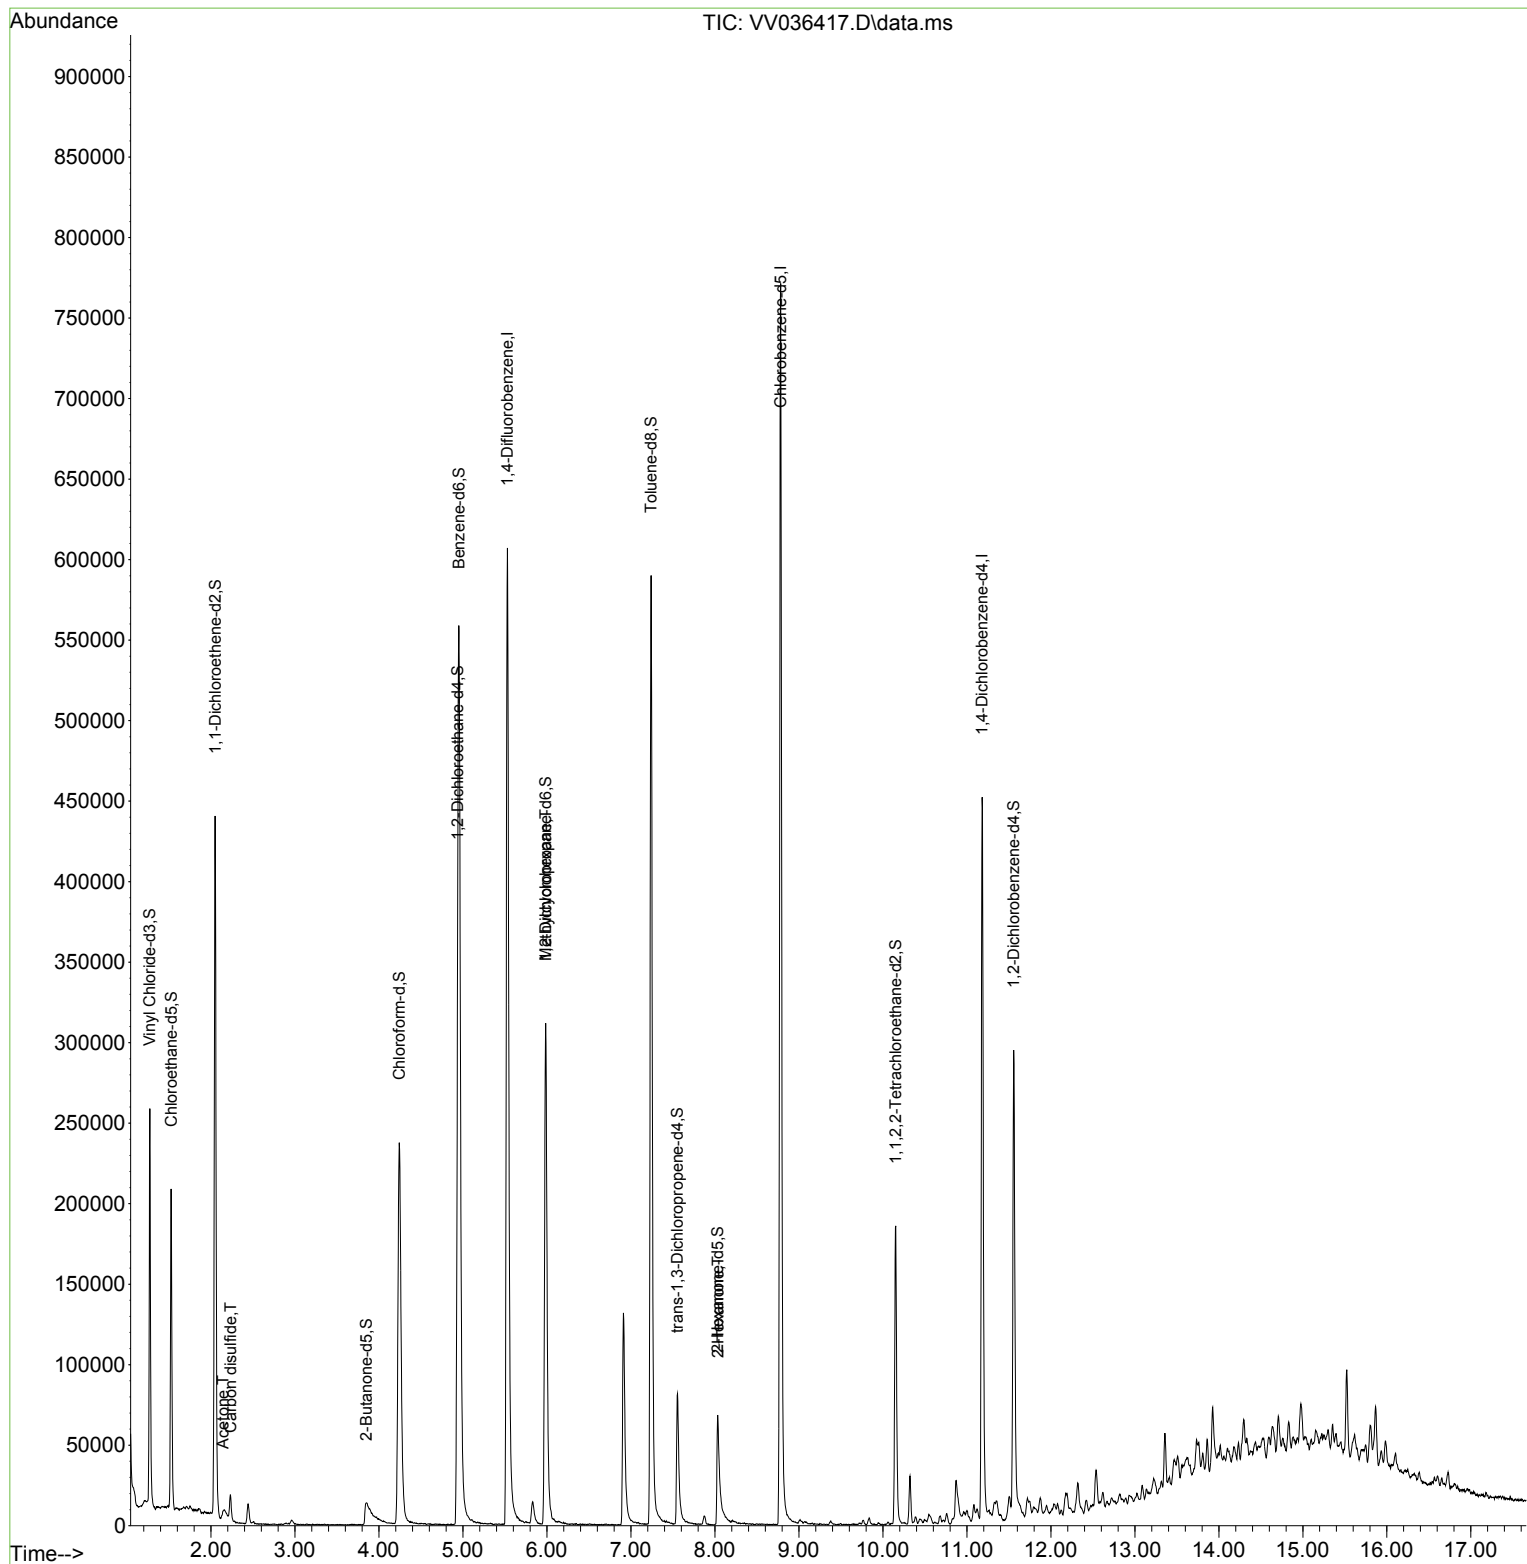

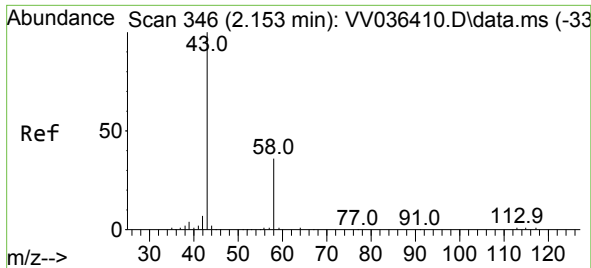

#13

Acetone

Concen: 1.701 ug/L

RT: 2.143 min Scan# 346

Delta R.T. -0.010 min

Lab File: VV036417.D

Acq: 02 Jul 2024 13:28

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 4935

Ion Ratio Lower Upper

43 100

58 92.6 0.0 0.6#

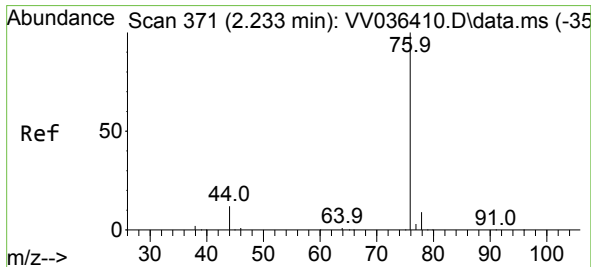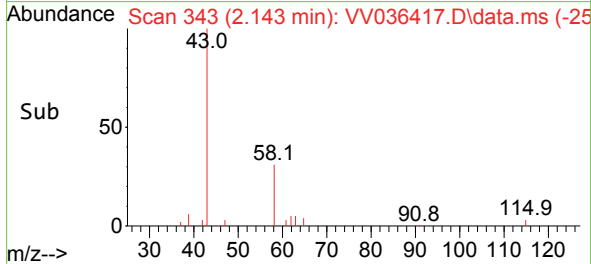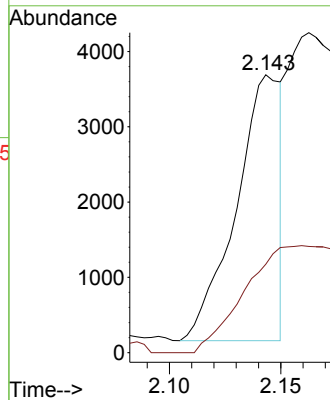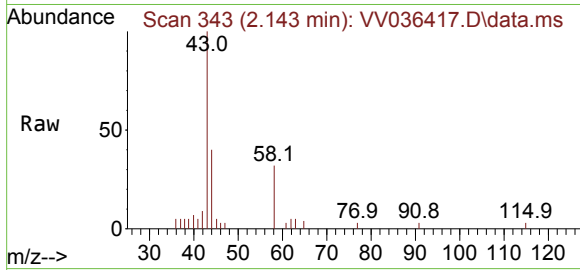

#14

Carbon disulfide

Concen: 0.651 ug/L

RT: 2.233 min Scan# 371

Delta R.T. 0.000 min

Lab File: VV036417.D




Acq: 02 Jul 2024 13:28


Tgt Ion: 76 Resp: 17640

Ion Ratio Lower Upper

76 100

78 9.9 7.4 11.2


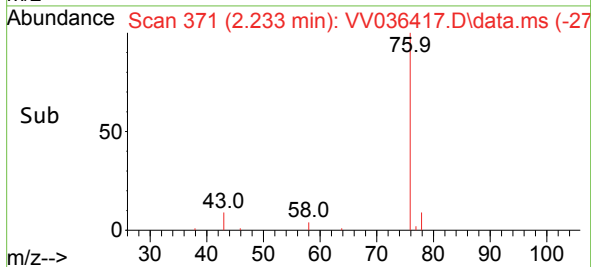
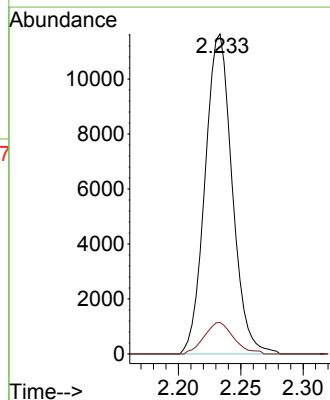
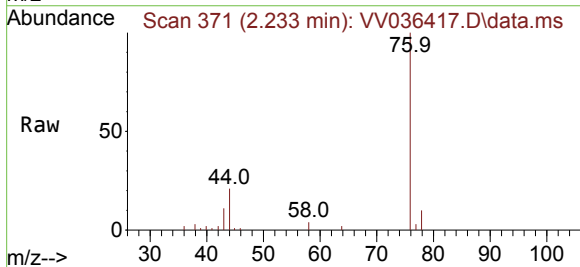


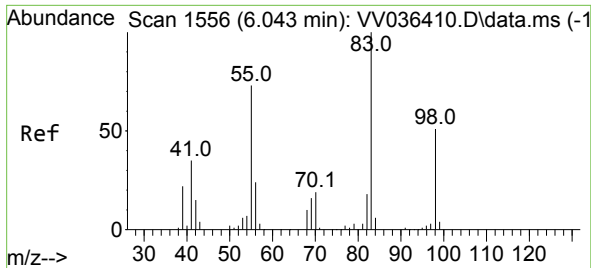

#35
Methylcyclohexane
Concen: 3.317 ug/L
RT: 5.986 min Scan# 11
Delta R.T. -0.058 min
Lab File: VV036417.D
Acq: 02 Jul 2024 13:28

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 83 Resp: 38737
Ion Ratio Lower Upper
83 100
55 0.7 56.0 84.0#
98 1.5 39.0 58.6#

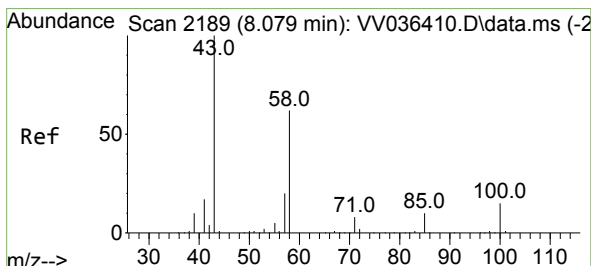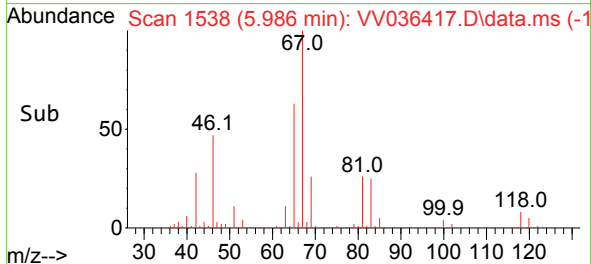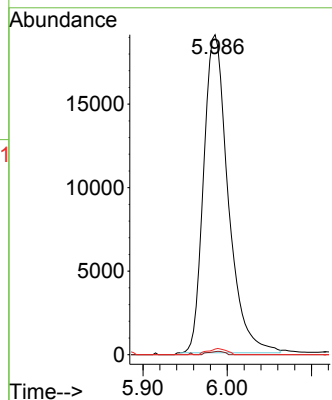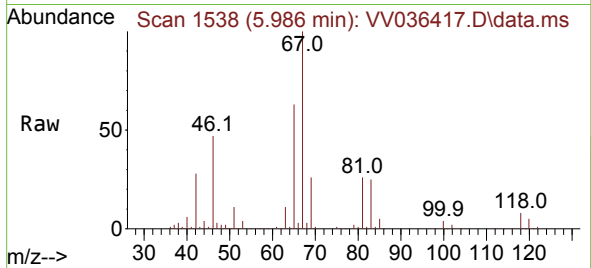

#48
2-Hexanone
Concen: 1.073 ug/L
RT: 8.037 min Scan# 2176
Delta R.T. -0.042 min
Lab File: VV036417.D
Acq: 02 Jul 2024 13:28

Tgt Ion: 43 Resp: 3229
Ion Ratio Lower Upper
43 100
58 20.5 48.5 72.7#
57 53.1 15.8 23.6#
100 6.8 10.9 16.3#

