




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070224\
 Data File : VV036423.D
 Acq On : 02 Jul 2024 15:46
 Operator : SY/MD
 Sample : P3087-21 RE
 Misc : 5.47g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4BR6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:13:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 03 05:08:41 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

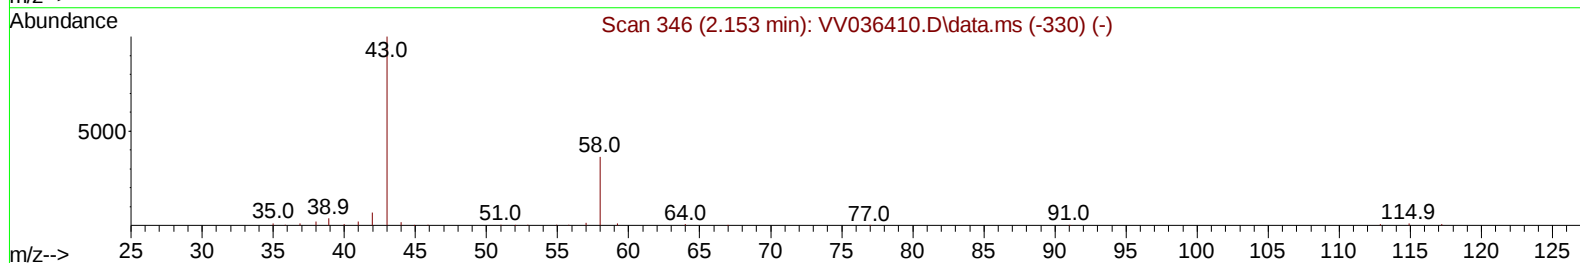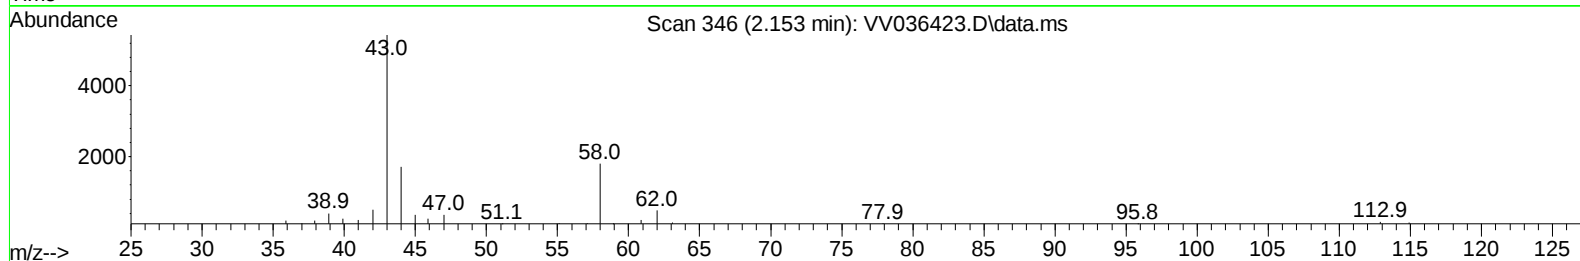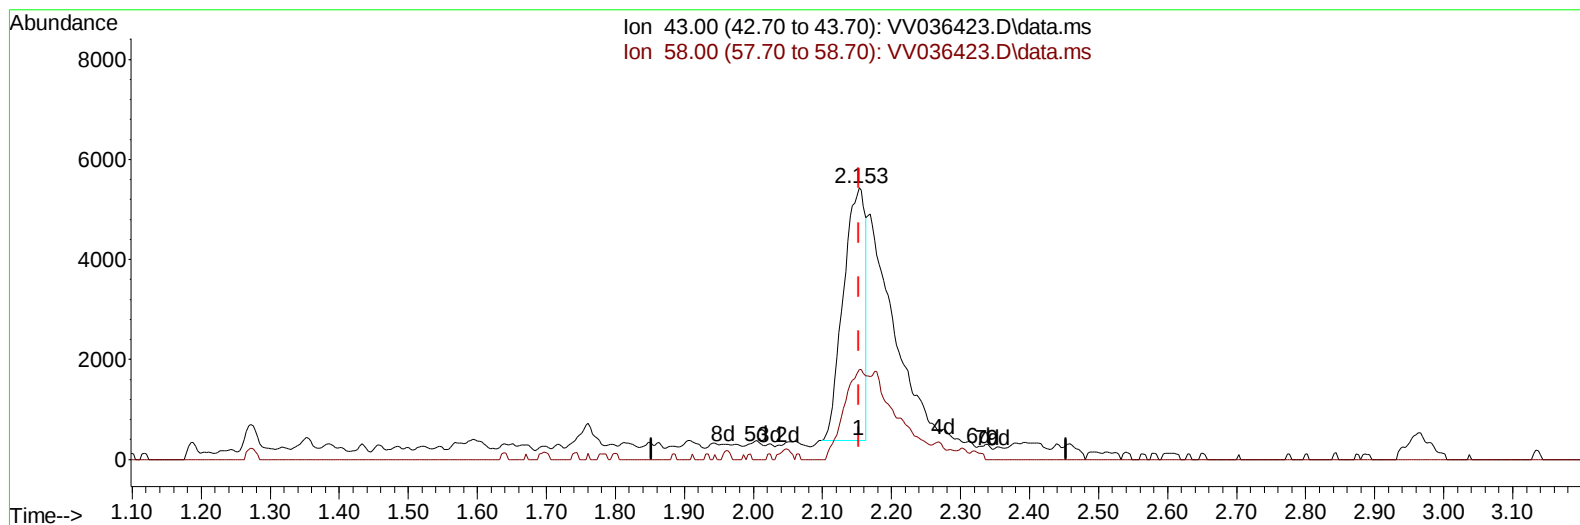

TIC: VV036423.D\data.ms

(13) Acetone (T)

2.153min (0.000) 3.99 ug/L

response 11027

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	0.30	41.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070224\
 Data File : VV036423.D
 Acq On : 02 Jul 2024 15:46
 Operator : SY/MD
 Sample : P3087-21 RE
 Misc : 5.47g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4BR6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:13:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 03 05:08:41 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

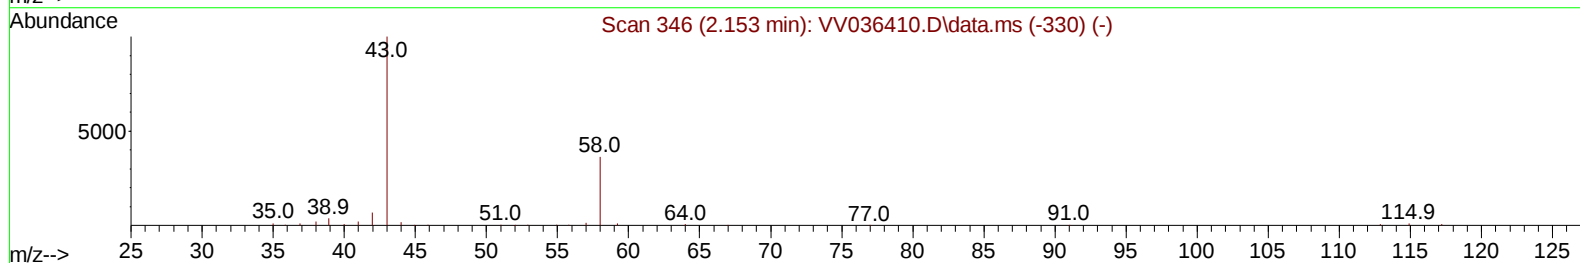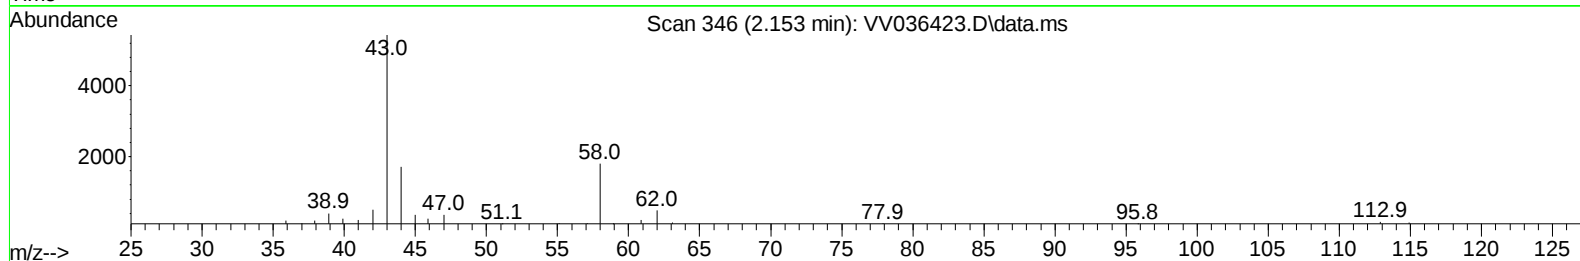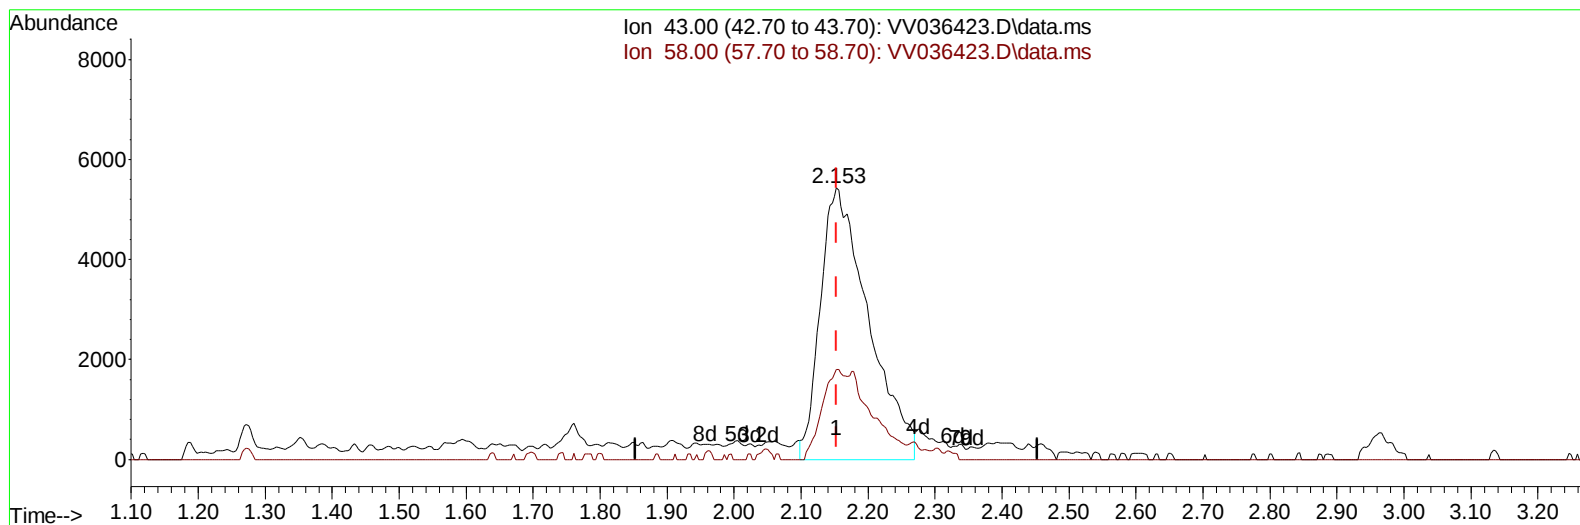

TIC: VV036423.D\data.ms

(13) Acetone (T)

2.153min (0.000) 9.78 ug/L m

response 27025

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	0.30	16.73#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070224\
 Data File : VV036423.D
 Acq On : 02 Jul 2024 15:46
 Operator : SY/MD
 Sample : P3087-21 RE
 Misc : 5.47g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4BR6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:13:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 03 05:08:41 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.529	114		518906	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117		379783	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		84487	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.272	65		143284	16.259	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	65.040%		
7) Chloroethane-d5	1.526	69		118144	16.784	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	67.120%		
11) 1,1-Dichloroethene-d2	2.050	65		63465	15.319	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	61.280%		
21) 2-Butanone-d5	3.854	46		30744	15.031	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135		Recovery =	30.060%		
24) Chloroform-d	4.243	84		239932	15.665	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	62.640%		
26) 1,2-Dichloroethane-d4	4.937	65		121987	14.934	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	59.720%#		
32) Benzene-d6	4.953	84		468979	21.875	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	87.520%		
36) 1,2-Dichloropropane-d6	5.986	67		139642	21.655	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	86.600%		
41) Toluene-d8	7.240	98		349852	18.099	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	72.400%		
43) trans-1,3-Dichloroprop...	7.555	79		40343	14.010	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	56.040%		
47) 2-Hexanone-d5	8.034	63		20140	19.566	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	39.140%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84		75258	14.237	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	56.960%		
66) 1,2-Dichlorobenzene-d4	11.561	152		49879	16.201	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	64.800%#		
Target Compounds							
13) Acetone	2.153	43		27025m	9.780	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070224\
Data File : VV036423.D
Acq On : 02 Jul 2024 15:46
Operator : SY/MD
Sample : P3087-21 RE
Misc : 5.47g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4BR6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 03 05:13:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 03 05:08:41 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

