

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070318\
 Data File : VV006546.D
 Acq On : 03 Jul 2018 12:05
 Operator : SY/MD
 Sample : J3834-01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEAN9

Quant Time: Jul 03 23:05:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 03 22:57:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	291239	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	268769	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	120407	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	90942	4.75	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.00%
7) Chloroethane-d5	1.58	69	76793	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.13	63	118251	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	3.96	46	238377	66.43	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	132.86%#
24) Chloroform-d	4.41	84	162802	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
26) 1,2-Dichloroethane-d4	5.09	65	83486	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.20%
32) Benzene-d6	5.11	84	344941	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.12	67	108557	5.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.20%
41) Toluene-d8	7.37	98	299469	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
43) trans-1,3-Dichloropropene-	7.67	79	32064	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.14	63	173851	57.13	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.26%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	63484	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	115867	5.18	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	7162	3.256 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070318\
Data File : VV006546.D
Acq On : 03 Jul 2018 12:05
Operator : SY/MD
Sample : J3834-01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEAN9

Quant Time: Jul 03 23:05:41 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 03 22:57:49 2018
Response via : Initial Calibration

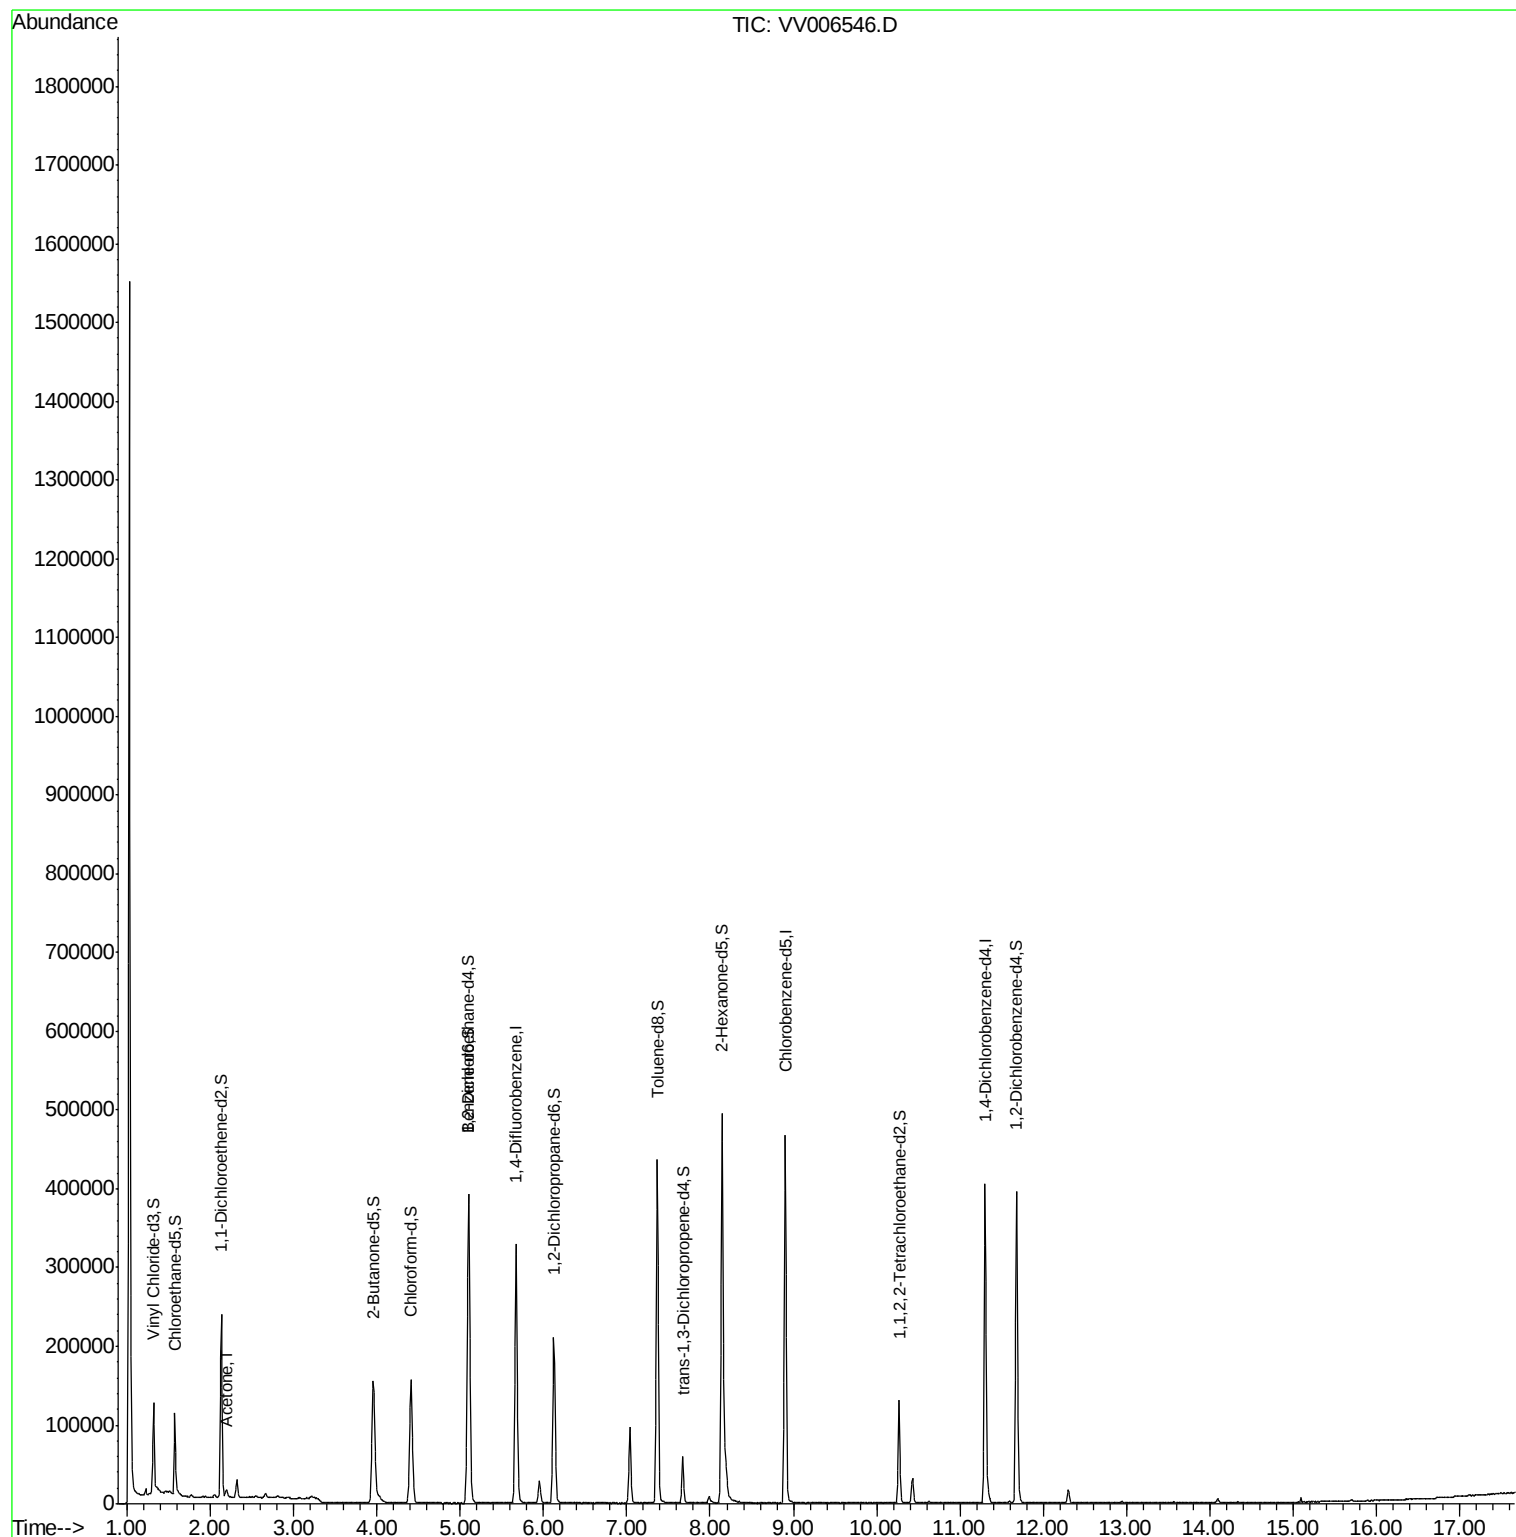

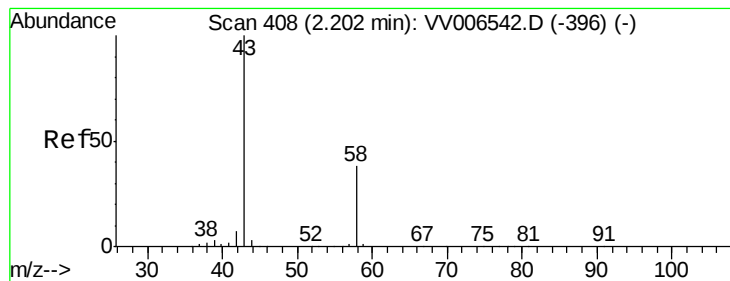

#13

Acetone

Concen: 3.256 ug/L

RT: 2.20 min Scan# 406

Delta R.T. -0.01 min

Lab File: VV006546.D

Acq: 03 Jul 2018 12:05


Instrument :
MSVOA_V
ClientSampleId :
BEAN9

Tot Ion: 43 Resp: 7162

Ion Ratio Lower Upper

43 100

58 41.0 0.0 77.4

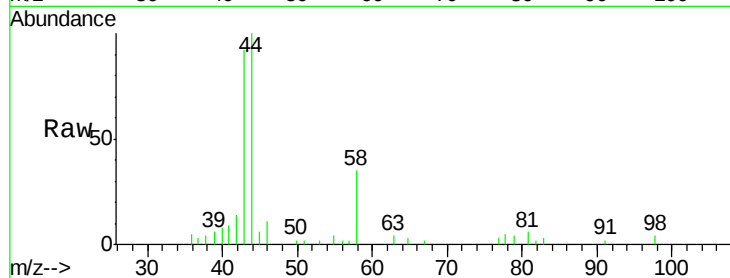

Abundance Ion 43.05 (42.75 to 43.75): VV0
Ion 58.05 (57.75 to 58.75): VV0

