

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070318\
 Data File : VV006548.D
 Acq On : 03 Jul 2018 13:27
 Operator : SY/MD
 Sample : J3792-23
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jul 03 23:18:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 03 22:57:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	276256	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	253800	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	112953	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	102827	5.66	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.20%
7) Chloroethane-d5	1.58	69	78747	5.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.60%
11) 1,1-Dichloroethene-d2	2.13	63	131556	4.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.80%
20) 2-Butanone-d5	3.96	46	204984	60.22	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.44%
24) Chloroform-d	4.41	84	157338	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
26) 1,2-Dichloroethane-d4	5.09	65	78855	5.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.80%
32) Benzene-d6	5.11	84	350711	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.20%
36) 1,2-Dichloropropane-d6	6.13	67	106457	5.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.20%
41) Toluene-d8	7.37	98	313858	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
43) trans-1,3-Dichloropropene-	7.67	79	32513	4.48	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.60%
46) 2-Hexanone-d5	8.14	63	146827	51.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.20%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	56791	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	112457	5.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.20%


Target Compounds					Ovalue
13) Acetone	2.20	43	5697	2.731 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070318\
Data File : VV006548.D
Acq On : 03 Jul 2018 13:27
Operator : SY/MD
Sample : J3792-23
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jul 03 23:18:26 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 03 22:57:49 2018
Response via : Initial Calibration

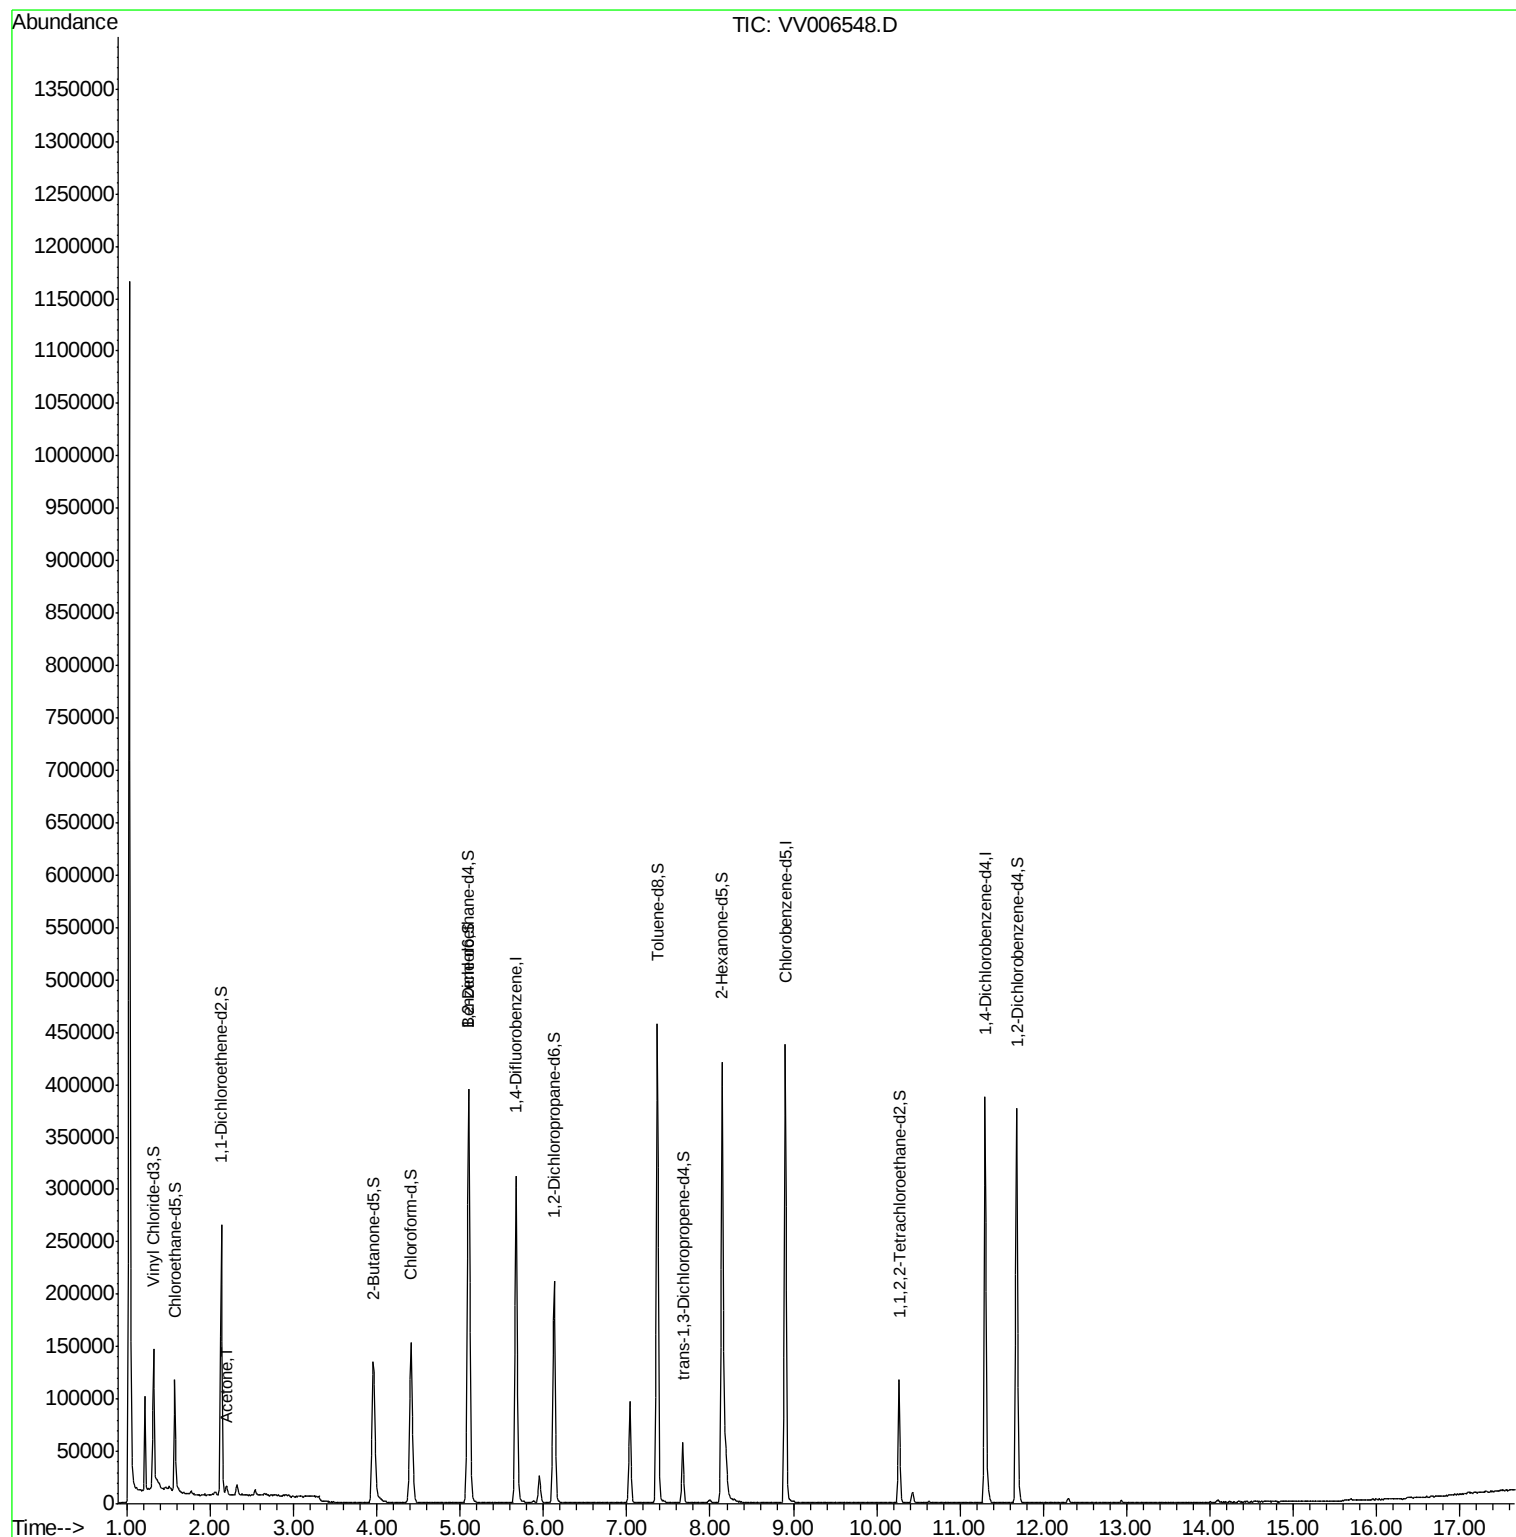

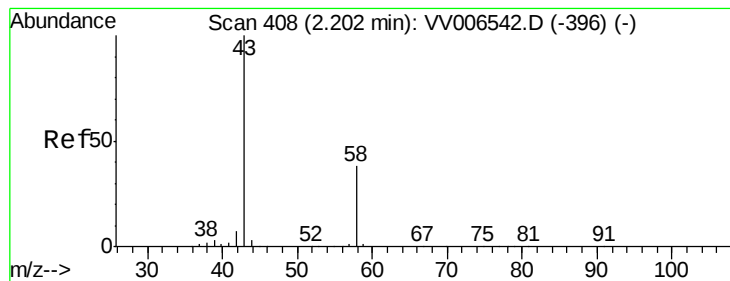

#13

Acetone

Concen: 2.731 ug/L

RT: 2.20 min Scan# 406

Delta R.T. -0.01 min

Lab File: VV006548.D

Acq: 03 Jul 2018 13:27

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tot Ion: 43 Resp: 5697

Ion Ratio Lower Upper

43 100

58 40.6 0.0 77.4

