

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070318\
 Data File : VV006549.D
 Acq On : 03 Jul 2018 13:55
 Operator : SY/MD
 Sample : J3834-04
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jul 03 23:19:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 03 22:57:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	271631	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	252491	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	111350	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	103390	5.79	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	115.80%
7) Chloroethane-d5	1.58	69	80895	5.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.40%
11) 1,1-Dichloroethene-d2	2.13	63	133735	4.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.60%
20) 2-Butanone-d5	3.95	46	211561	63.21	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.42%
24) Chloroform-d	4.41	84	159612	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
26) 1,2-Dichloroethane-d4	5.09	65	80248	5.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.60%
32) Benzene-d6	5.11	84	354925	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.00%
36) 1,2-Dichloropropane-d6	6.13	67	106872	5.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.00%
41) Toluene-d8	7.37	98	314619	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.00%
43) trans-1,3-Dichloropropene-	7.67	79	32526	4.51	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.20%
46) 2-Hexanone-d5	8.14	63	155121	54.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.52%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	62497	5.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	113043	5.46	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.20%


Target Compounds					Ovalue
13) Acetone	2.20	43	6338	3.090 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070318\
Data File : VV006549.D
Acq On : 03 Jul 2018 13:55
Operator : SY/MD
Sample : J3834-04
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jul 03 23:19:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 03 22:57:49 2018
Response via : Initial Calibration

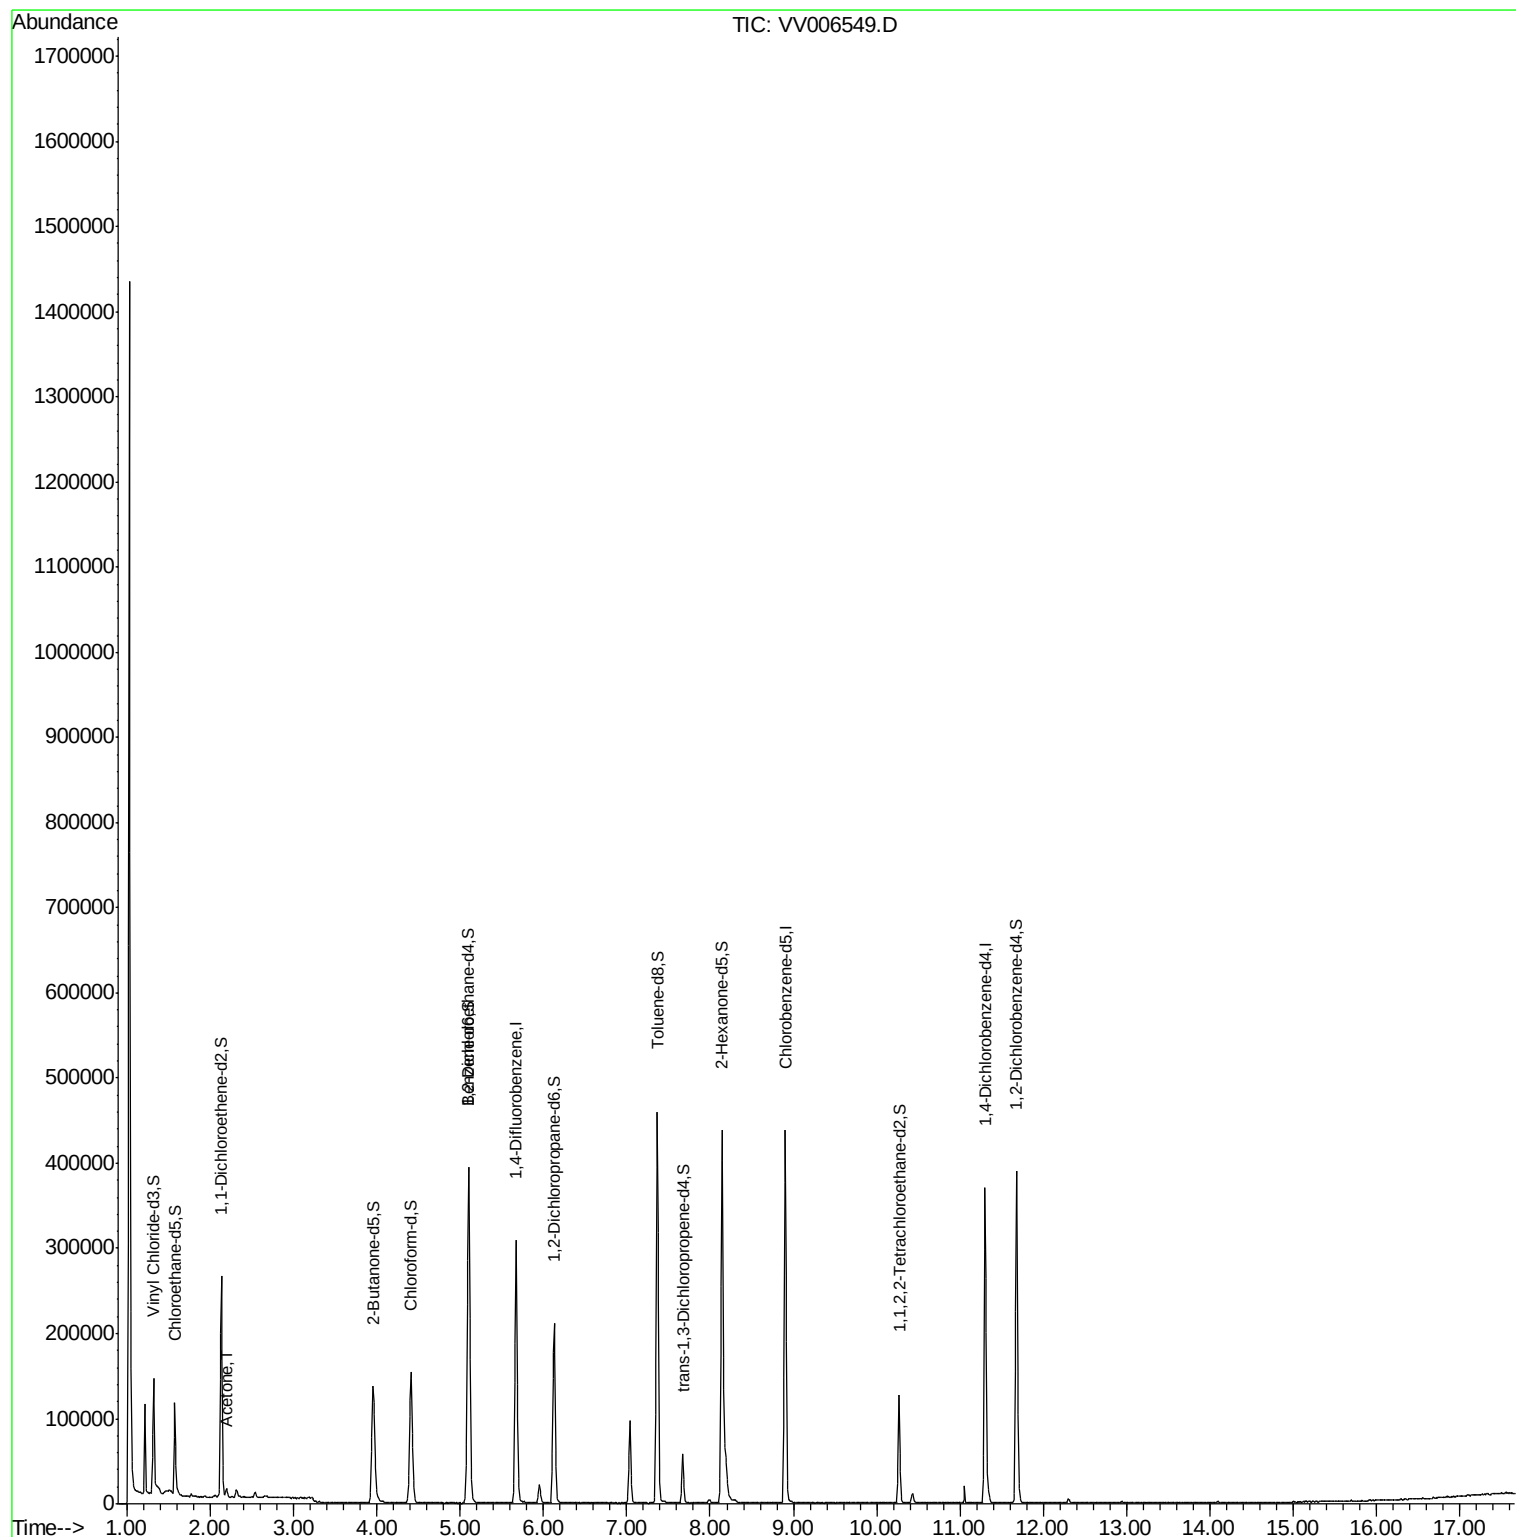

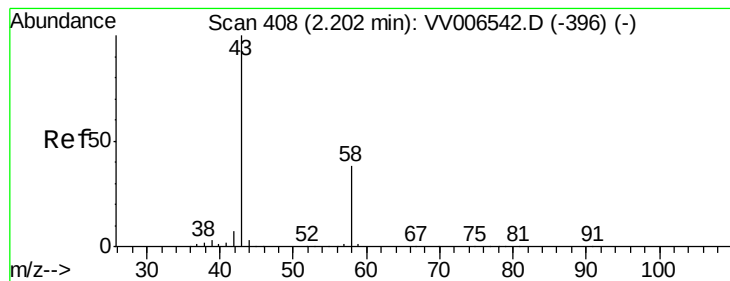

#13

Acetone

Concen: 3.090 ug/L

RT: 2.20 min Scan# 406

Delta R.T. -0.01 min

Lab File: VV006549.D

Acq: 03 Jul 2018 13:55

Instrument :

MSVOA_V

ClientSampleId :


VHBLK01

Tot Ion: 43 Resp: 6338

Ion Ratio Lower Upper

43 100

58 41.8 0.0 77.4

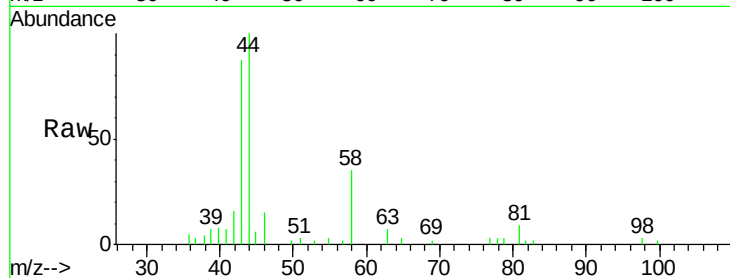

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

5000

4000

3000

2000

1000

0

2.15 2.20 2.25

Time-->

