

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070318\
 Data File : VV006546.D
 Acq On : 03 Jul 2018 12:05
 Operator : SY/MD
 Sample : J3834-01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEAN9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.029	26	43	76	rBV	1551669	1875180	100.00%	19.285%
2	1.318	124	133	144	rBV	115887	139376	7.43%	1.433%
3	1.575	206	213	222	rBV	102203	119001	6.35%	1.224%
4	2.132	376	386	397	rBV	232529	322726	17.21%	3.319%
5	2.318	436	444	455	rVB	21433	33288	1.78%	0.342%
6	3.958	937	954	993	rBV	155236	414624	22.11%	4.264%
7	4.408	1076	1094	1118	rBV	157462	378166	20.17%	3.889%
8	5.103	1292	1310	1333	rBV2	392806	901530	48.08%	9.272%
9	5.672	1471	1487	1515	rBV	327972	640677	34.17%	6.589%
10	5.951	1563	1574	1595	rVB	27292	53181	2.84%	0.547%
11	6.125	1612	1628	1652	rBV	210562	429783	22.92%	4.420%
12	7.038	1899	1912	1935	rBV	96318	168930	9.01%	1.737%
13	7.366	1999	2014	2034	rBV	436221	748453	39.91%	7.697%
14	7.672	2098	2109	2125	rBV	58808	94816	5.06%	0.975%
15	8.144	2240	2256	2293	rBV2	494111	1023233	54.57%	10.523%
16	8.903	2479	2492	2522	rBV	467825	752667	40.14%	7.741%
17	10.270	2904	2917	2939	rBV	130206	205420	10.95%	2.113%
18	10.430	2955	2967	2985	rBV	31785	53351	2.85%	0.549%
19	11.302	3226	3238	3265	rBV	404659	684792	36.52%	7.043%
20	11.678	3343	3355	3378	rBV	394869	656914	35.03%	6.756%
21	12.302	3538	3549	3560	rBV2	16554	27376	1.46%	0.282%


Sum of corrected areas: 9723484

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070318\
Data File : VV006546.D
Acq On : 03 Jul 2018 12:05
Operator : SY/MD
Sample : J3834-01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEAN9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

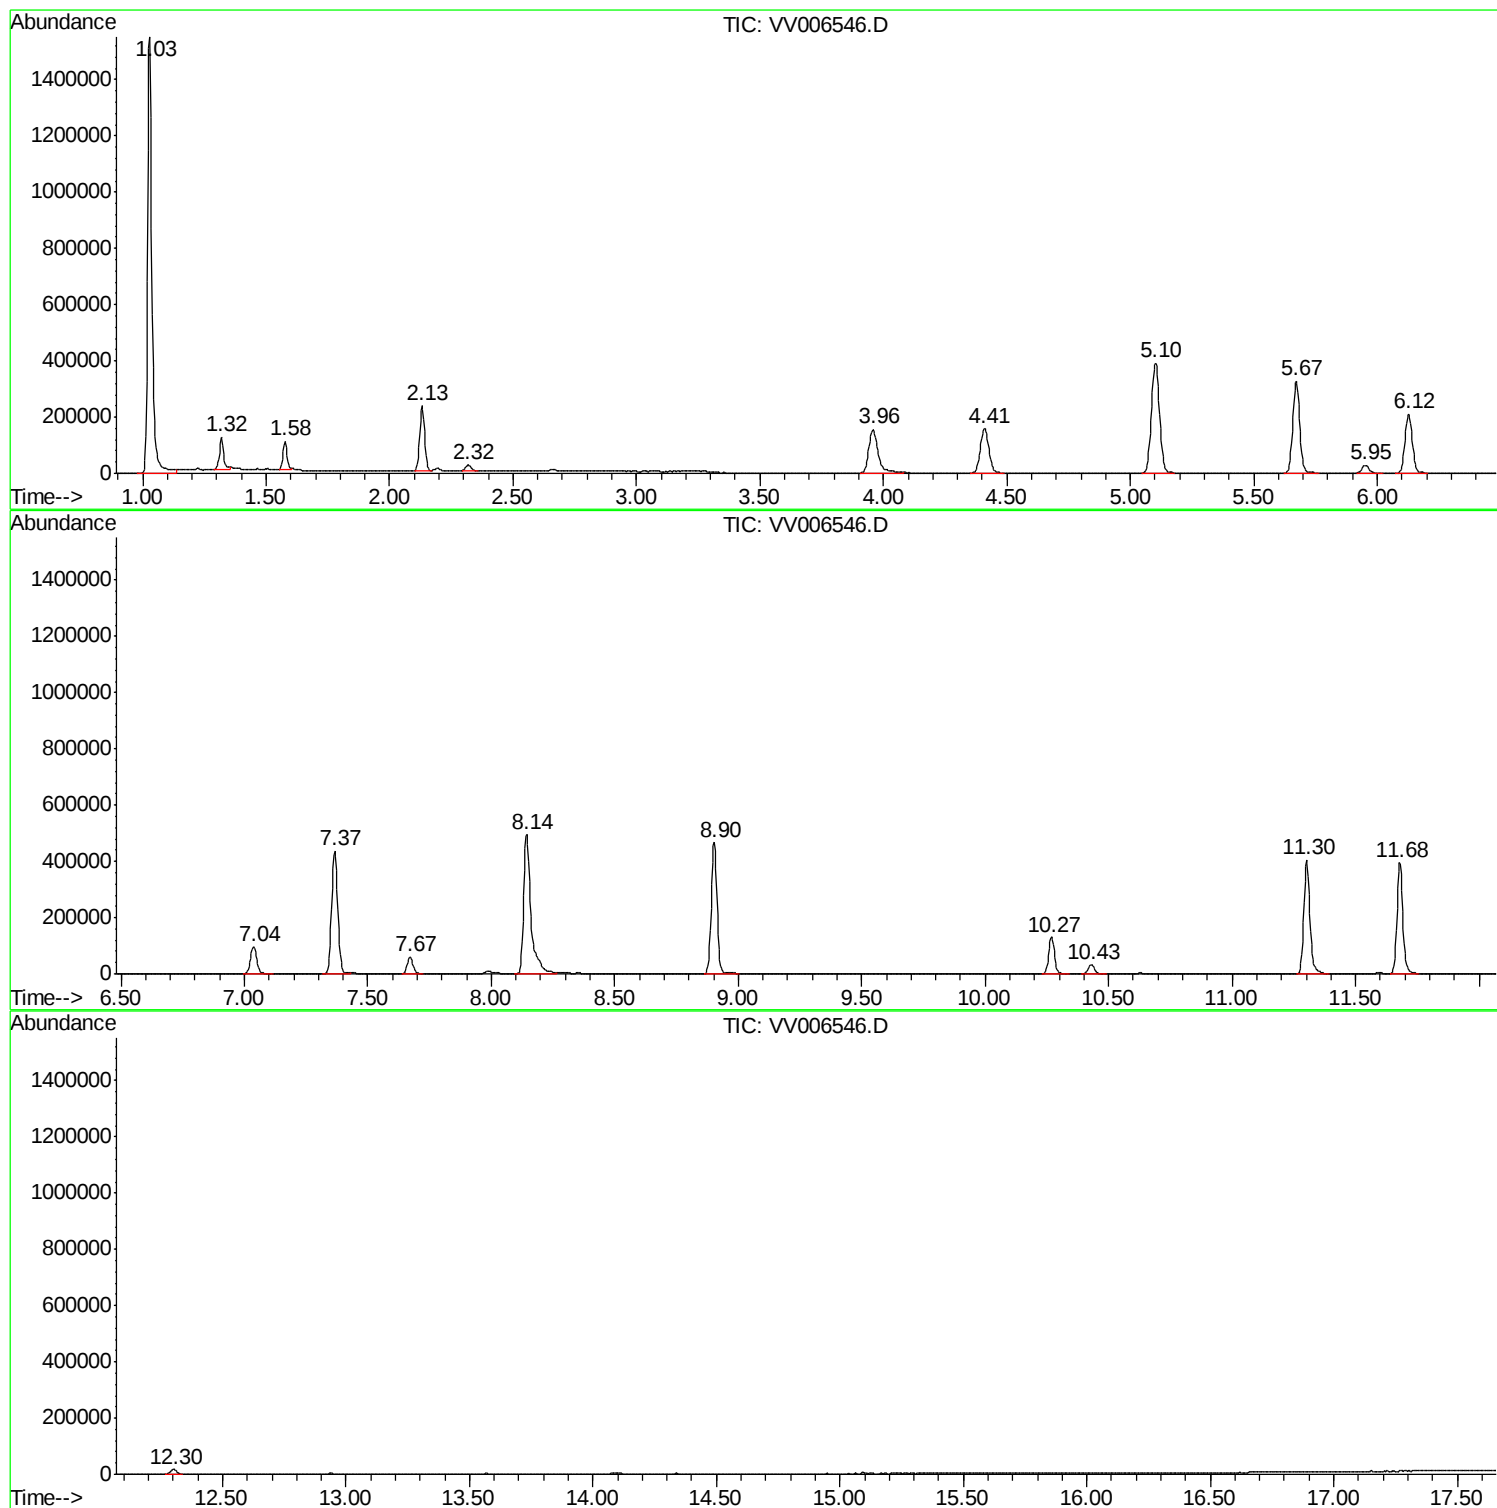

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV070318\
Data_File : VV006546.D
Acq_On : 03-Jul-2018 12:055
Operator : SY/MDD
Sample : J3834-011
Misc : 25 mL/MSVOA_V/WATER
ALS_Vial : 1 Sample_Multiplier: 11

Instrument :
MSVOA_V
ClientSampleId :
BEAN9

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.MM
Quant_Title : TRACE_VOA_SOM01_00

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
