


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070318\
Data File : VV006541.D
Acq On : 03 Jul 2018 08:47
Operator : SY/MD
Sample : BFB65
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jul 05 12:04:44 2018

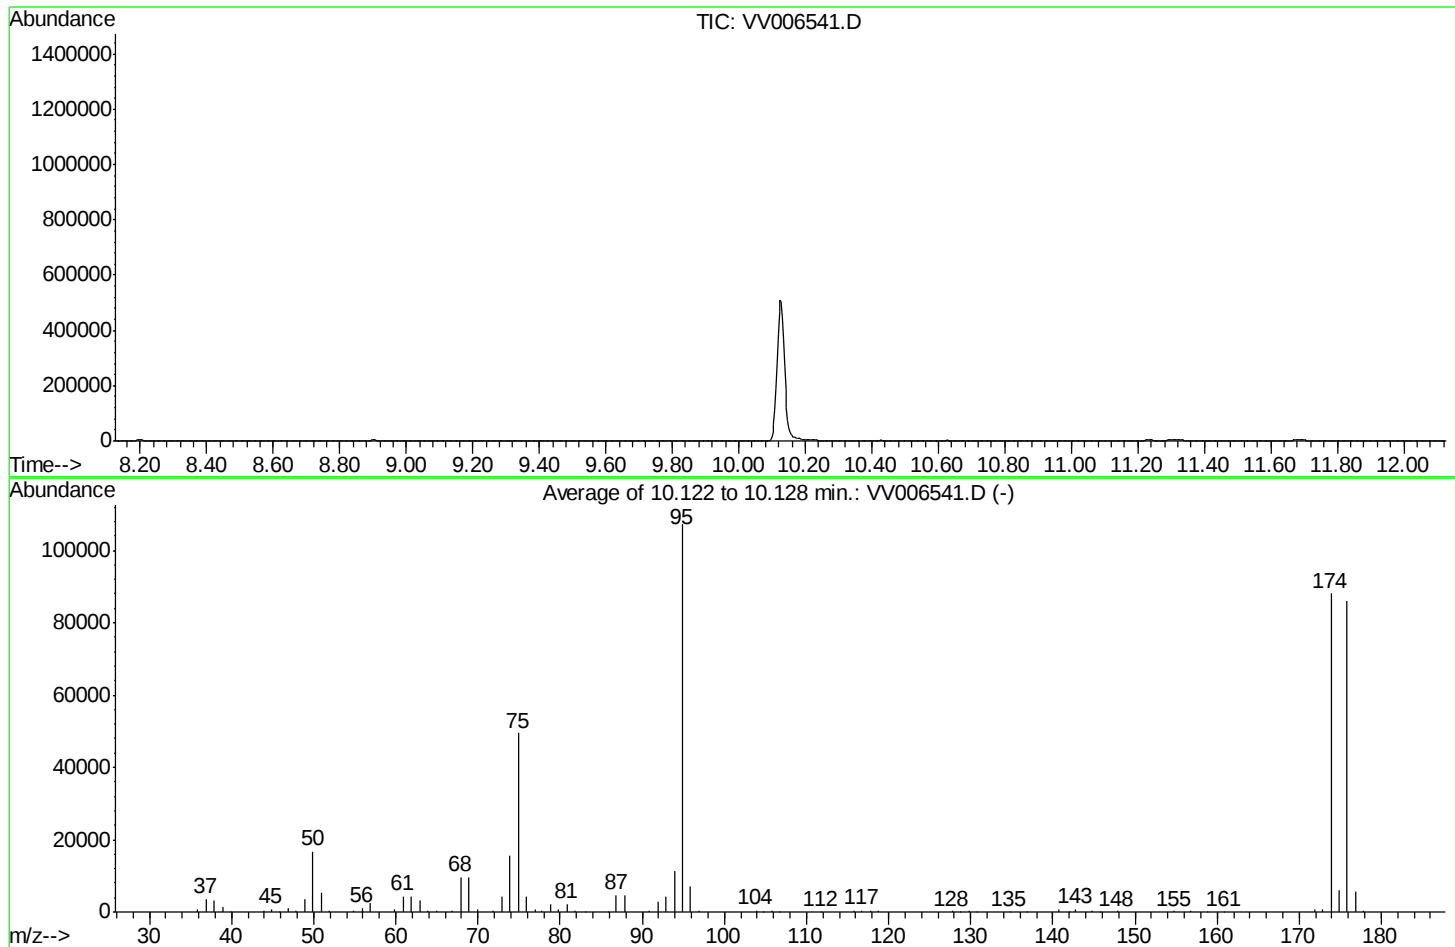

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	16701	PASS
75	95	30	80	46.1	49464	PASS
95	95	100	100	100.0	107237	PASS
96	95	5	9	6.5	6967	PASS
173	174	0.00	2	0.8	716	PASS
174	95	50	120	82.2	88098	PASS
175	174	5	9	7.0	6201	PASS
176	174	95	101	97.7	86042	PASS
177	176	5	9	6.7	5734	PASS

m/z	Abundance
35.90	588.0
36.90	3429.0
37.90	3214.0
38.90	1520.0
40.00	337.0
43.90	1152.0
44.80	664.0
45.80	141.0
46.90	1078.0
47.80	499.0
48.90	3287.0
49.90	16087.0
50.90	5053.0
51.80	206.0
54.90	288.0
55.90	1055.0
56.90	2268.0
59.90	838.0
60.90	4286.0
61.90	3968.0
62.90	3098.0
63.90	417.0
64.90	497.0
66.80	187.0
67.90	9281.0
68.90	9045.0
69.90	753.0
71.80	444.0
72.90	4158.0
73.90	15269.0
74.90	47312.0
75.90	4135.0
76.90	621.0
77.70	450.0
78.80	2098.0
79.80	706.0
80.80	2115.0
81.80	505.0
85.80	139.0
86.80	4511.0
87.90	4463.0
90.80	330.0
91.90	2666.0
92.90	4086.0
93.90	10927.0
94.90	101880.0
95.90	6810.0
96.90	196.0
103.90	361.0
104.70	154.0
105.80	345.0
106.70	107.0
115.80	245.0
116.70	477.0
117.80	290.0
118.80	465.0
127.70	287.0
128.70	151.0
129.80	269.0
134.80	163.0
136.80	120.0
140.80	718.0
142.80	768.0
144.80	167.0
145.80	162.0
147.80	194.0
154.90	207.0
156.80	196.0
158.80	129.0
171.80	616.0
172.90	672.0
173.90	80904.0
174.90	5922.0
175.80	79736.0
176.90	5416.0
177.80	209.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	635.0
36.90	3767.0
37.90	3346.0
38.90	1542.0
40.00	346.0
43.90	1168.0
44.80	755.0
45.80	153.0
46.90	1187.0
47.80	546.0
48.90	3620.0
49.90	17320.0
50.90	5349.0
51.90	224.0
54.90	253.0
55.90	1158.0
56.90	2500.0
59.90	900.0
60.90	4600.0
61.90	4253.0
62.90	3428.0
63.90	460.0
64.90	522.0
66.90	202.0
67.90	9952.0
68.90	9760.0
69.90	802.0
71.90	482.0
72.90	4482.0
73.90	16247.0
74.90	51160.0
75.90	4424.0
76.90	674.0
77.70	470.0
78.90	2289.0
79.80	811.0
80.80	2212.0
81.80	549.0
85.80	130.0
86.80	4779.0
87.90	4799.0
90.80	305.0
91.90	2910.0
92.90	4429.0
93.90	12033.0
94.90	111008.0
95.90	7217.0
97.00	206.0
103.90	466.0
104.70	161.0
105.80	387.0
106.80	125.0
115.80	284.0
116.70	553.0
117.80	277.0
118.70	508.0
127.80	328.0
128.70	169.0
129.80	278.0
130.80	115.0
134.80	187.0
136.80	138.0
140.80	776.0
142.80	815.0
144.80	208.0
145.70	177.0
147.80	233.0
154.80	216.0
156.80	193.0
158.70	114.0
160.90	118.0
171.80	718.0
172.90	739.0
173.90	91192.0
174.90	6388.0
175.80	88992.0
176.90	5944.0
177.80	219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.80	641.0
36.90	3713.0
37.90	3193.0
38.90	1472.0
40.00	340.0
43.90	1113.0
44.80	722.0
45.80	134.0
46.90	1101.0
47.80	541.0
48.90	3541.0
49.90	16696.0
50.90	5238.0
51.90	241.0
54.90	204.0
55.90	1214.0
56.90	2526.0
59.90	843.0
60.90	4356.0
61.90	4202.0
62.90	3386.0
63.90	440.0
64.90	521.0
66.90	197.0
67.90	9623.0
68.90	9531.0
69.90	794.0
71.90	480.0
72.90	4308.0
73.90	15729.0
74.90	49920.0
75.90	4174.0
77.00	686.0
77.70	431.0
78.90	2269.0
79.80	835.0
80.90	2148.0
81.80	541.0
83.00	102.0
85.80	123.0
86.80	4737.0
87.80	4710.0
90.80	272.0
91.90	2785.0
92.90	4369.0
93.90	11582.0
94.90	108824.0
95.90	6875.0
97.00	211.0
103.90	449.0
104.80	151.0
105.80	392.0
106.80	119.0
111.80	110.0
115.90	312.0
116.80	593.0
117.70	285.0
118.70	505.0
127.80	327.0
128.80	150.0
129.70	301.0
130.80	122.0
134.80	182.0
136.80	153.0
140.80	770.0
141.90	104.0
142.80	874.0
144.90	209.0
145.80	148.0
147.90	230.0
154.70	223.0
156.80	188.0
160.90	113.0
171.90	784.0
172.90	737.0
173.90	92200.0
174.90	6293.0
175.80	89400.0
176.90	5842.0
177.80	193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Scan 2858 (10.080 min): VV006541.D
BFB65

m/z	Abundance
39.90	197.0
43.90	752.0


Instrument :
MSVOA_V
ClientSampleId :
BFB65

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070318\
Data File : VV006541.D
Acq On : 03 Jul 2018 08:47
Operator : SY/MD
Sample : BFB65
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jul 05 12:04:44 2018

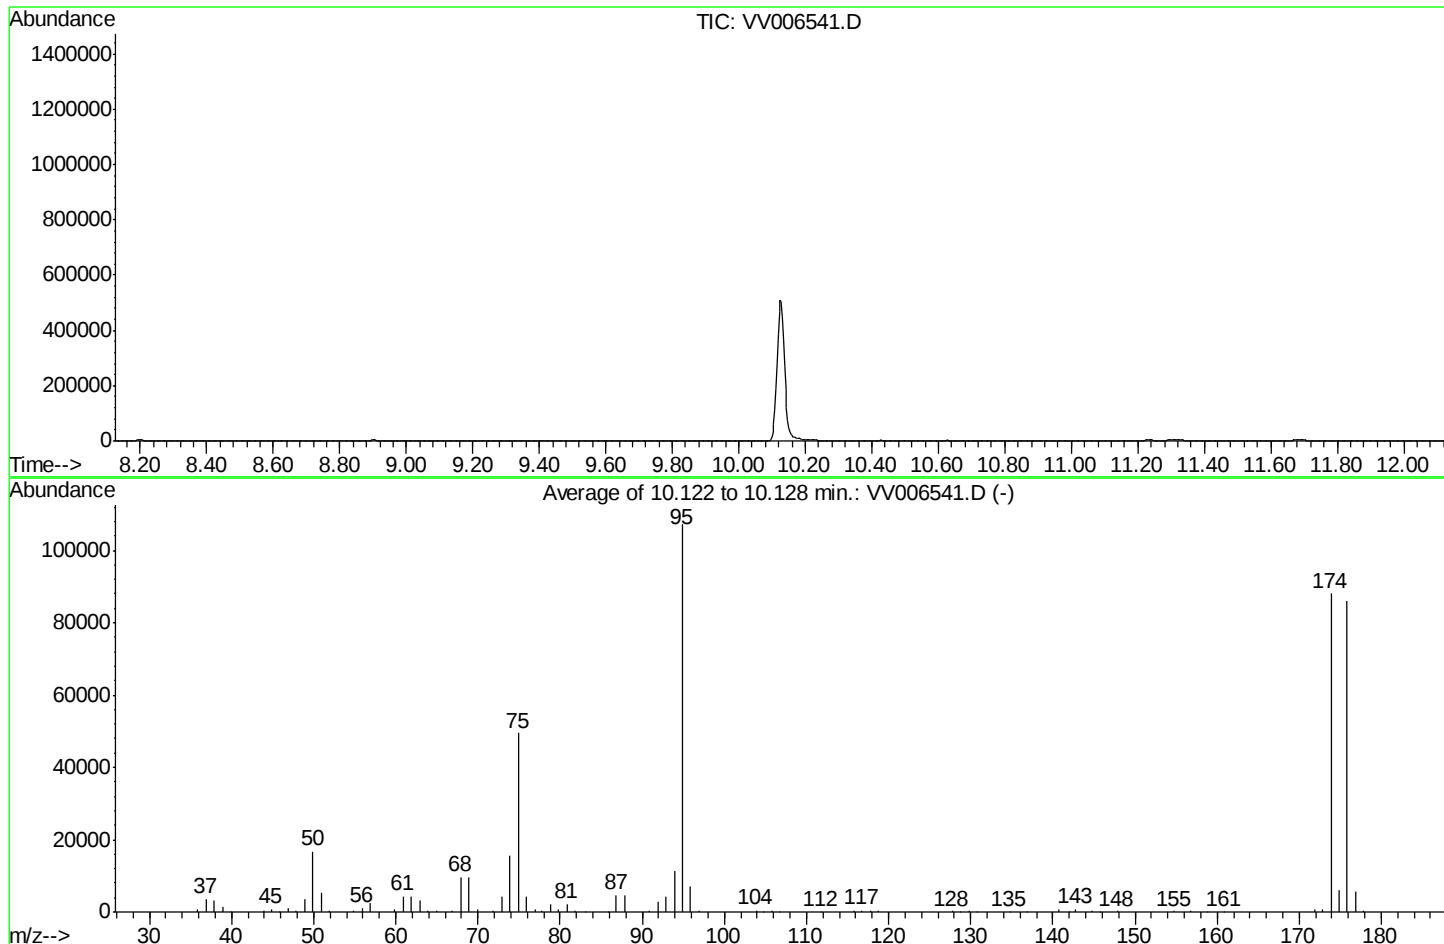

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	16701	PASS
75	95	30	80	46.1	49464	PASS
95	95	100	100	100.0	107237	PASS
96	95	5	9	6.5	6967	PASS
173	174	0.00	2	0.8	716	PASS
174	95	50	120	82.2	88098	PASS
175	174	5	9	7.0	6201	PASS
176	174	95	101	97.7	86042	PASS
177	176	5	9	6.7	5734	PASS