

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070324\
 Data File : VV036443.D
 Acq On : 03 Jul 2024 14:56
 Operator : SY/MD
 Sample : P3100-10
 Misc : 5.10g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 04 02:11:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 04 02:05:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	595532	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	516095	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	174208	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	174944	17.297	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.200%
7) Chloroethane-d5	1.526	69	143642	17.781	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.120%
11) 1,1-Dichloroethene-d2	2.050	65	78232	16.454	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.800%
21) 2-Butanone-d5	3.834	46	6173	2.630	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	5.260%#
24) Chloroform-d	4.243	84	277483	15.785	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	63.160%
26) 1,2-Dichloroethane-d4	4.937	65	136784	14.591	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	58.360%#
32) Benzene-d6	4.953	84	536328	18.409	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.640%
36) 1,2-Dichloropropane-d6	5.985	67	163429	18.650	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.600%
41) Toluene-d8	7.239	98	434307	16.534	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	66.120%
43) trans-1,3-Dichloroprop...	7.554	79	46475	11.876	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	47.520%
47) 2-Hexanone-d5	8.037	63	17221	12.311	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	24.620%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	93435	13.007	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	52.040%
66) 1,2-Dichlorobenzene-d4	11.557	152	106475	16.772	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	67.080%#
Target Compounds						Qvalue
16) Methylene chloride	2.442	84	47328	4.037	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070324\
Data File : VV036443.D
Acq On : 03 Jul 2024 14:56
Operator : SY/MD
Sample : P3100-10
Misc : 5.10g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jul 04 02:11:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 04 02:05:51 2024
Response via : Initial Calibration

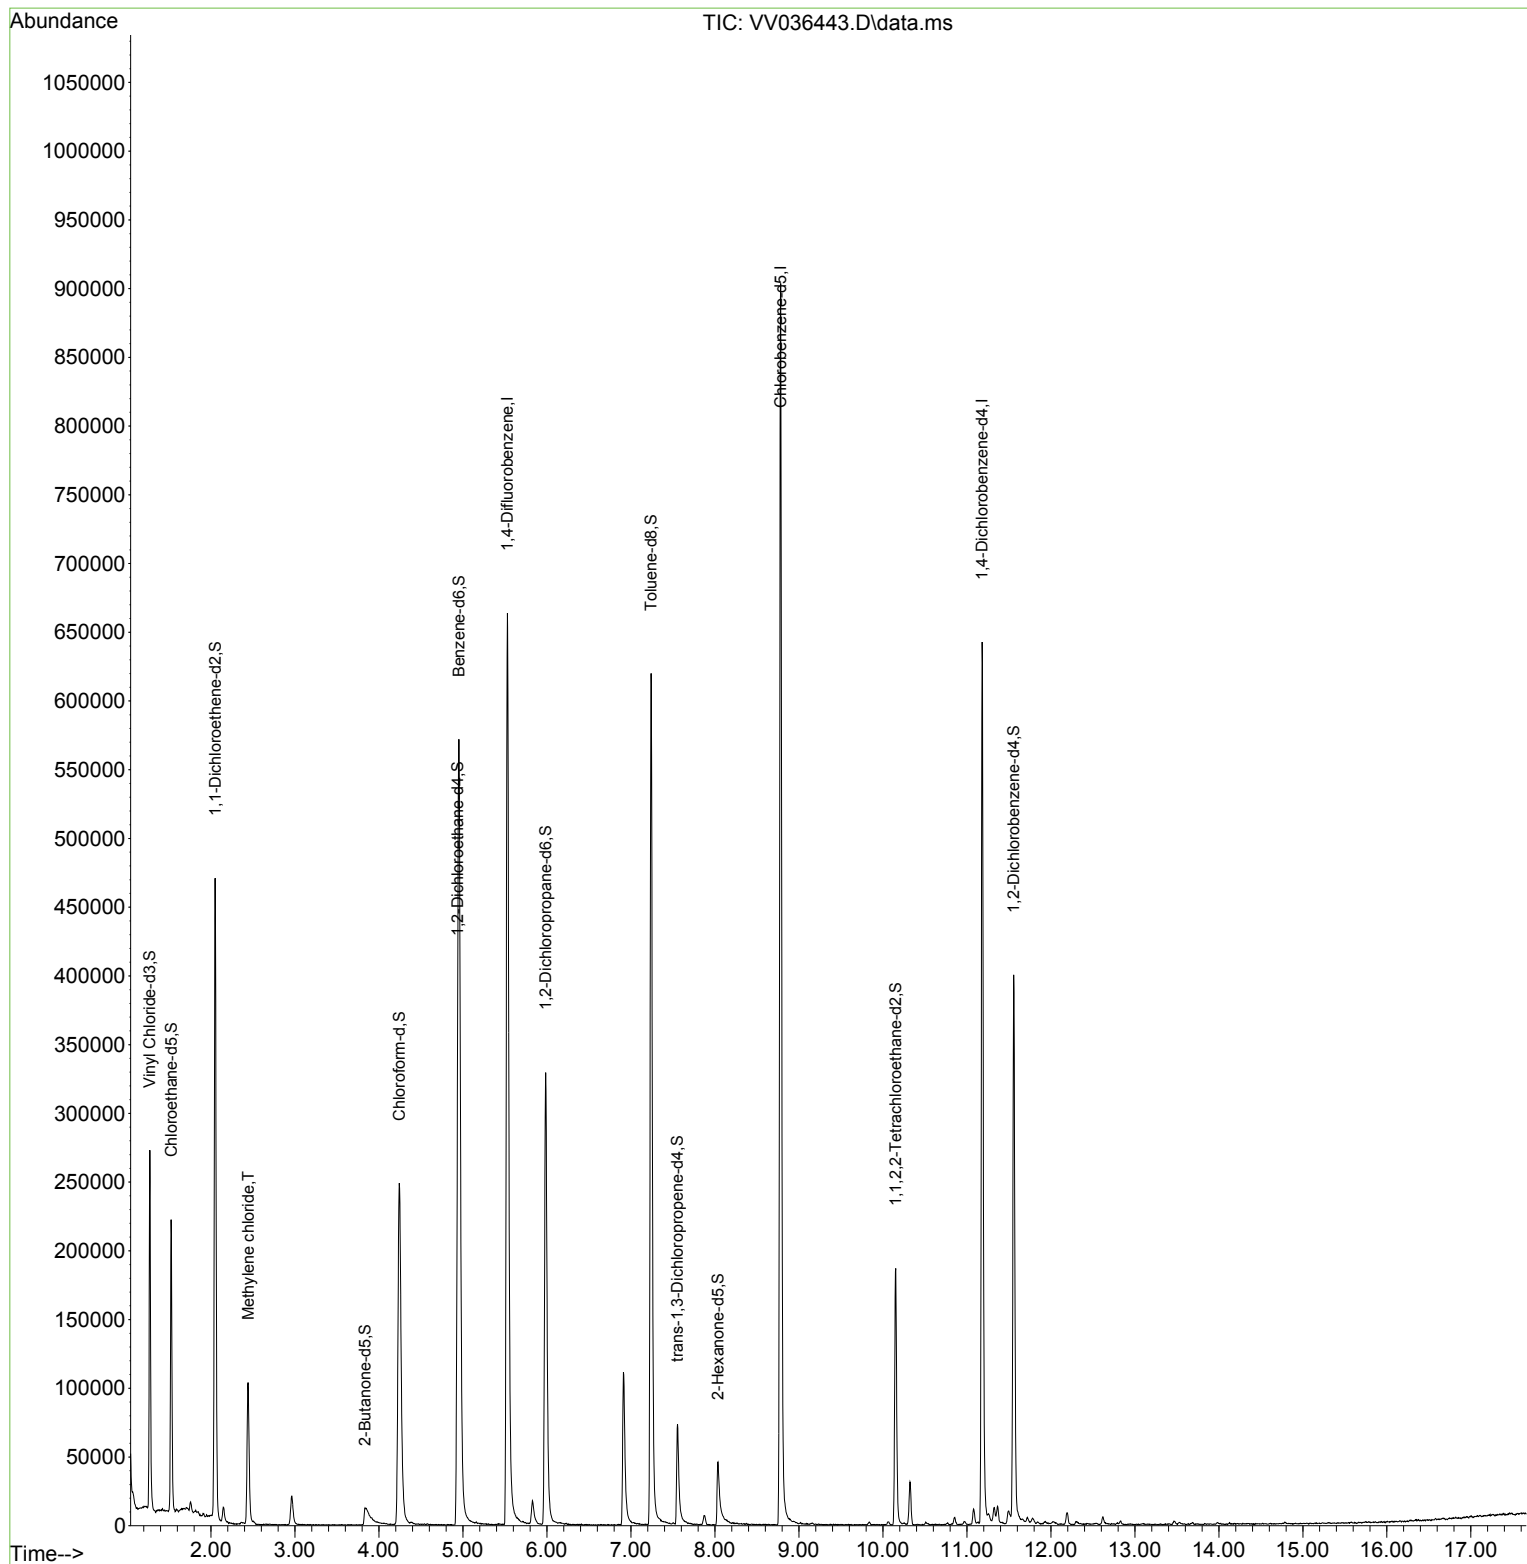

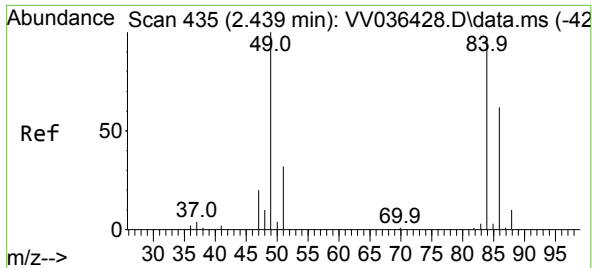

#16
Methylene chloride
Concen: 4.037 ug/L
RT: 2.442 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV036443.D
Acq: 03 Jul 2024 14:56

Instrument :
MSVOA_V
ClientSampleId :

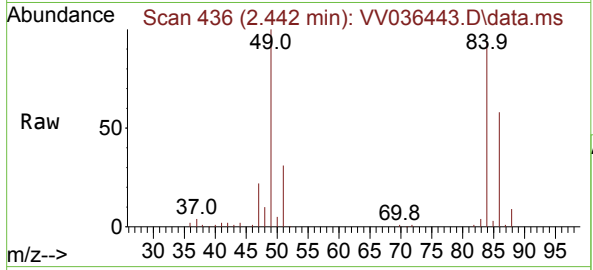

Tgt Ion:	84	Resp:	47328
Ion	Ratio	Lower	Upper
84	100		
86	62.1	45.6	84.8
49	106.4	75.7	140.5

