

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070524\
 Data File : VV036459.D
 Acq On : 05 Jul 2024 10:44
 Operator : SY/MD
 Sample : P3100-21RE
 Misc : 5.59g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4D38RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Title : VOC Analysis

Signal : TIC: VV036459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	95	rVB	444690	483033	16.49%	2.310%
2	1.526	144	151	180	rVB	419826	503858	17.20%	2.409%
3	2.053	304	315	335	rBV	831601	1206661	41.20%	5.770%
4	2.442	427	436	452	rVB2	14629	24631	0.84%	0.118%
5	2.815	549	552	557	rBV2	209	209	0.01%	0.001%
6	2.835	557	558	559	rBV2	151	48	0.00%	0.000%
7	2.963	591	598	612	rVB5	2727	5484	0.19%	0.026%
8	3.159	657	659	660	rVB5	322	86	0.00%	0.000%
9	3.304	702	704	707	rVB2	167	67	0.00%	0.000%
10	3.320	707	709	718	rVB2	310	215	0.01%	0.001%
11	3.368	722	724	726	rVB	164	65	0.00%	0.000%
12	3.384	726	729	732	rBV	308	205	0.01%	0.001%
13	3.433	742	744	749	rVB2	281	165	0.01%	0.001%
14	3.523	771	772	773	rBV2	124	29	0.00%	0.000%
15	3.597	792	795	799	rVB2	283	174	0.01%	0.001%
16	3.616	799	801	804	rBV	250	155	0.01%	0.001%
17	3.648	808	811	813	rBV	191	100	0.00%	0.000%
18	3.719	831	833	839	rVB2	371	287	0.01%	0.001%
19	3.751	839	843	845	rBV	256	211	0.01%	0.001%
20	3.806	852	860	892	rBV2	29408	94728	3.23%	0.453%
21	4.243	980	996	1028	rBV	459008	1182931	40.39%	5.656%
22	4.645	1119	1121	1122	rVB	613	165	0.01%	0.001%
23	4.661	1122	1126	1128	rBV3	281	157	0.01%	0.001%
24	4.799	1168	1169	1171	rVB	194	45	0.00%	0.000%
25	4.818	1171	1175	1178	rVB3	299	218	0.01%	0.001%
26	4.841	1178	1182	1185	rBV3	412	308	0.01%	0.001%
27	4.857	1185	1187	1190	rBV2	327	191	0.01%	0.001%
28	4.876	1190	1193	1195	rBV	378	194	0.01%	0.001%
29	4.950	1200	1216	1258	rBV2	1045594	2608867	89.07%	12.474%
30	5.529	1384	1396	1438	rBV	1310691	2595925	88.63%	12.412%
31	5.825	1480	1488	1508	rVB	30622	65721	2.24%	0.314%
32	5.982	1524	1537	1568	rBV	578281	1195246	40.81%	5.715%
33	6.317	1639	1641	1642	rBV2	407	155	0.01%	0.001%
34	6.346	1648	1650	1651	rBV2	308	91	0.00%	0.000%
35	6.375	1657	1659	1664	rVB2	669	427	0.01%	0.002%
36	6.400	1664	1667	1670	rVB2	470	256	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070524\
 Data File : VV036459.D
 Acq On : 05 Jul 2024 10:44
 Operator : SY/MD
 Sample : P3100-21RE
 Misc : 5.59g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4D38RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Title : VOC Analysis

37	6.461	1684	1686	1690	rBV	268	168	0.01%	0.001%
38	6.503	1697	1699	1700	rBV	290	109	0.00%	0.001%
39	6.551	1712	1714	1715	rBV	143	53	0.00%	0.000%
40	6.558	1715	1716	1718	rVV	349	143	0.00%	0.001%
41	6.571	1718	1720	1721	rVB2	202	54	0.00%	0.000%
42	6.584	1722	1724	1725	rBV2	123	29	0.00%	0.000%
43	6.654	1744	1746	1749	rBV	290	182	0.01%	0.001%
44	6.683	1754	1755	1757	rBV	112	23	0.00%	0.000%
45	6.693	1757	1758	1759	rVB	109	21	0.00%	0.000%
46	6.703	1759	1761	1762	rBV	316	137	0.00%	0.001%
47	6.802	1789	1792	1795	rBV3	286	156	0.01%	0.001%
48	6.825	1795	1799	1802	rBV	303	208	0.01%	0.001%
49	6.841	1802	1804	1805	rBV	135	50	0.00%	0.000%
50	6.908	1814	1825	1858	rBV	259277	494917	16.90%	2.366%
51	7.240	1916	1928	1959	rBV	1382591	2349486	80.21%	11.234%
52	7.551	2016	2025	2049	rBV	159262	293010	10.00%	1.401%
53	7.876	2118	2126	2135	rBV3	5813	9048	0.31%	0.043%
54	7.976	2155	2157	2160	rBV2	501	287	0.01%	0.001%
55	7.992	2160	2162	2164	rVB	230	108	0.00%	0.001%
56	8.027	2164	2173	2210	rBV	116035	250119	8.54%	1.196%
57	8.513	2321	2324	2328	rVB4	480	356	0.01%	0.002%
58	8.567	2339	2341	2346	rVB3	662	364	0.01%	0.002%
59	8.629	2358	2360	2362	rBV2	412	130	0.00%	0.001%
60	8.641	2362	2364	2368	rVB	317	186	0.01%	0.001%
61	8.725	2388	2390	2395	rBV3	386	184	0.01%	0.001%
62	8.780	2395	2407	2437	rBV	1831125	2929039	100.00%	14.005%
63	9.288	2563	2565	2568	rBV3	635	414	0.01%	0.002%
64	9.355	2582	2586	2591	rVB3	689	507	0.02%	0.002%
65	9.439	2607	2612	2616	rBV5	482	515	0.02%	0.002%
66	9.497	2624	2630	2636	rBV5	773	979	0.03%	0.005%
67	9.574	2652	2654	2656	rVB2	530	191	0.01%	0.001%
68	9.696	2689	2692	2695	rBV	206	135	0.00%	0.001%
69	9.776	2716	2717	2719	rBV	190	57	0.00%	0.000%
70	9.831	2729	2734	2737	rBV3	535	579	0.02%	0.003%
71	9.915	2757	2760	2763	rBV3	365	235	0.01%	0.001%
72	10.018	2787	2792	2794	rBV3	312	267	0.01%	0.001%
73	10.050	2800	2802	2803	rBV3	738	344	0.01%	0.002%
74	10.149	2822	2833	2858	rBV	327951	522982	17.86%	2.501%
75	10.326	2879	2888	2901	rVB2	19757	32250	1.10%	0.154%
76	10.378	2901	2904	2905	rBV	272	126	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070524\
 Data File : VV036459.D
 Acq On : 05 Jul 2024 10:44
 Operator : SY/MD
 Sample : P3100-21RE
 Misc : 5.59g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4D38RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Title : VOC Analysis

77	10.471	2930	2933	2935	rBV	240	178	0.01%	0.001%
78	10.484	2935	2937	2938	rBV2	356	135	0.00%	0.001%
79	10.574	2962	2965	2968	rBV3	271	206	0.01%	0.001%
80	10.632	2982	2983	2987	rVB	276	126	0.00%	0.001%
81	10.706	3004	3006	3008	rBV2	333	159	0.01%	0.001%
82	10.741	3015	3017	3018	rBV	356	149	0.01%	0.001%
83	10.802	3033	3036	3040	rBV3	577	517	0.02%	0.002%
84	10.854	3044	3052	3057	rBV4	3178	4739	0.16%	0.023%
85	11.082	3116	3123	3131	rBV4	6736	9175	0.31%	0.044%
86	11.182	3143	3154	3188	rBV	1622980	2435624	83.15%	11.646%
87	11.558	3260	3271	3300	rVB	1011905	1573436	53.72%	7.523%
88	12.194	3461	3469	3479	rVB2	10396	15732	0.54%	0.075%
89	12.300	3495	3502	3505	rBV6	3191	4221	0.14%	0.020%
90	12.445	3544	3547	3549	rBV2	849	538	0.02%	0.003%
91	12.587	3588	3591	3592	rBV	622	281	0.01%	0.001%
92	12.616	3592	3600	3609	rVV5	5325	8974	0.31%	0.043%
93	12.789	3650	3654	3656	rBV4	641	492	0.02%	0.002%




Sum of corrected areas: 20914138

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070524\
Data File : VV036459.D
Acq On : 05 Jul 2024 10:44
Operator : SY/MD
Sample : P3100-21RE
Misc : 5.59g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4D38RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

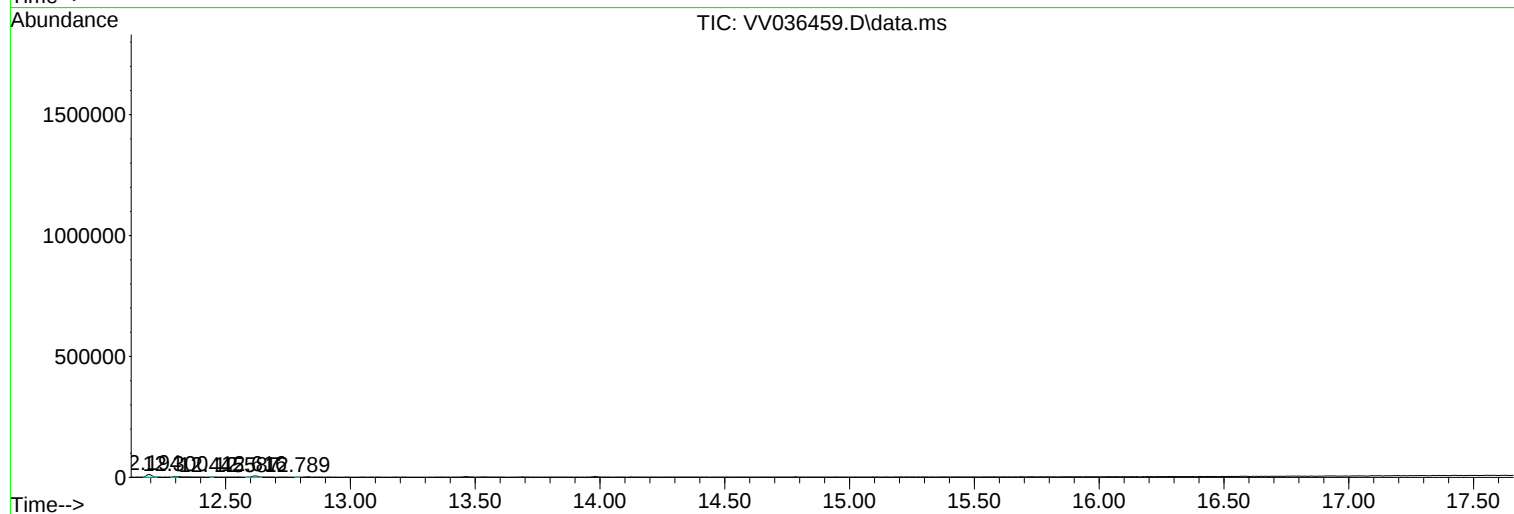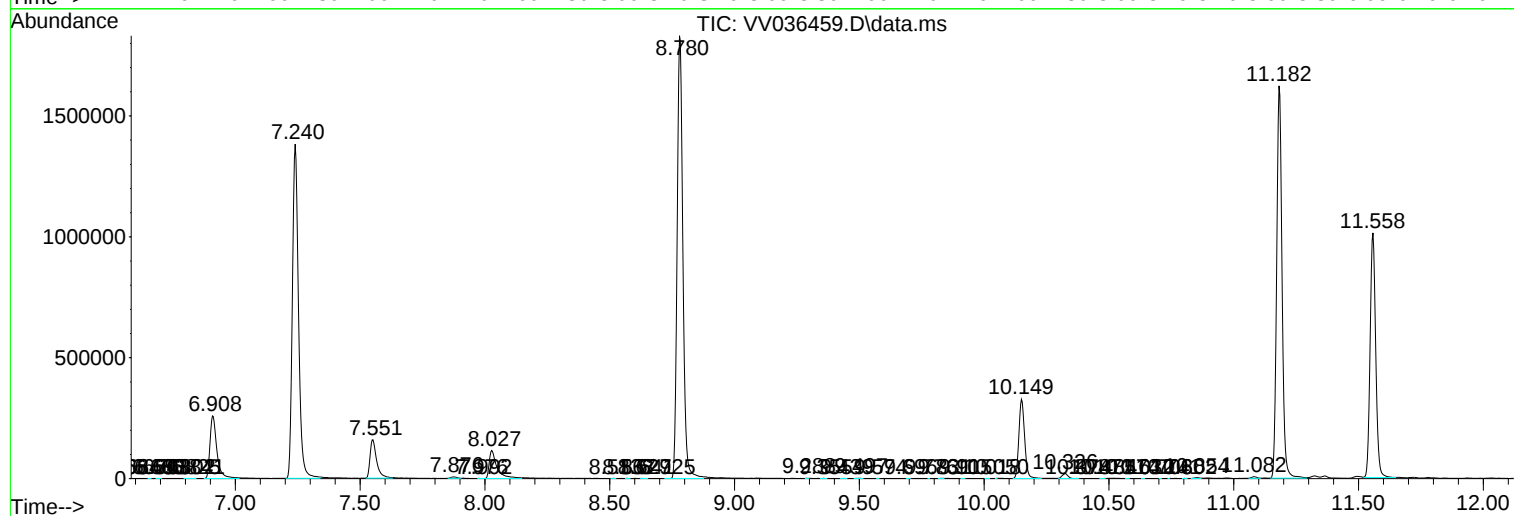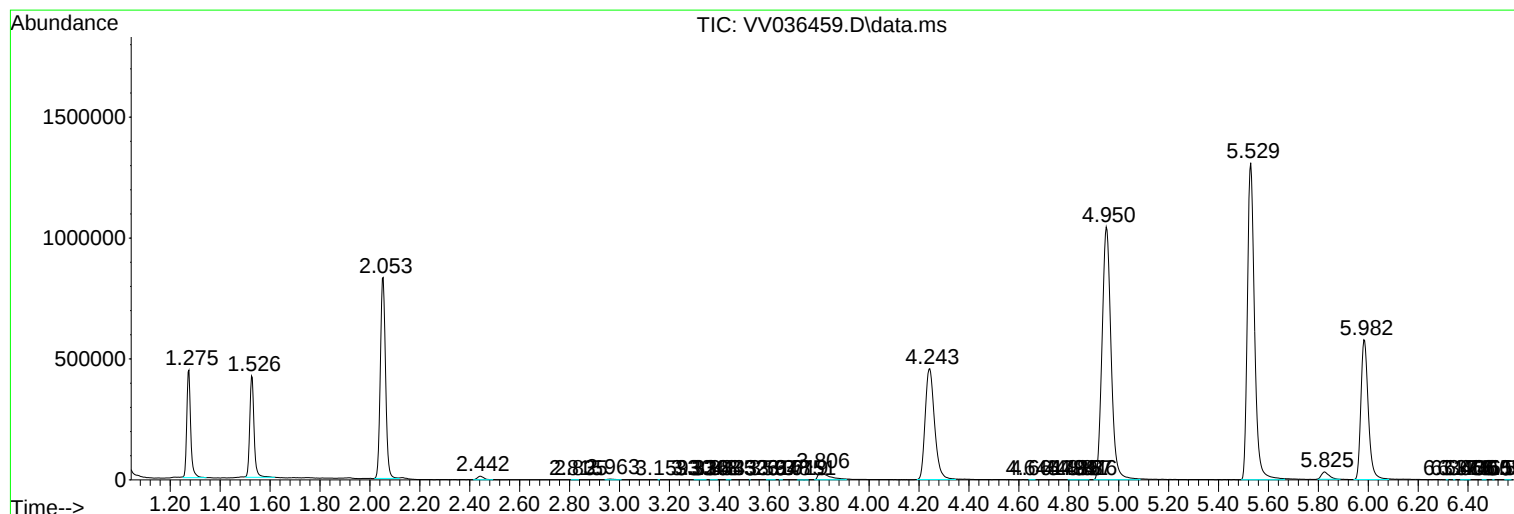

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070524\
Data File : VV036459.D
Acq On : 05 Jul 2024 10:44
Operator : SY/MD
Sample : P3100-21RE
Misc : 5.59g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4D38RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070524\
Data File : VV036459.D
Acq On : 05 Jul 2024 10:44
Operator : SY/MD
Sample : P3100-21RE
Misc : 5.59g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4D38RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc