


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070524\
Data File : VV036453.D
Acq On : 05 Jul 2024 07:50
Operator : SY/MD
Sample : BFB336
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB327

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Title : VOC Analysis
Last Update : Sat Jul 06 01:35:25 2024

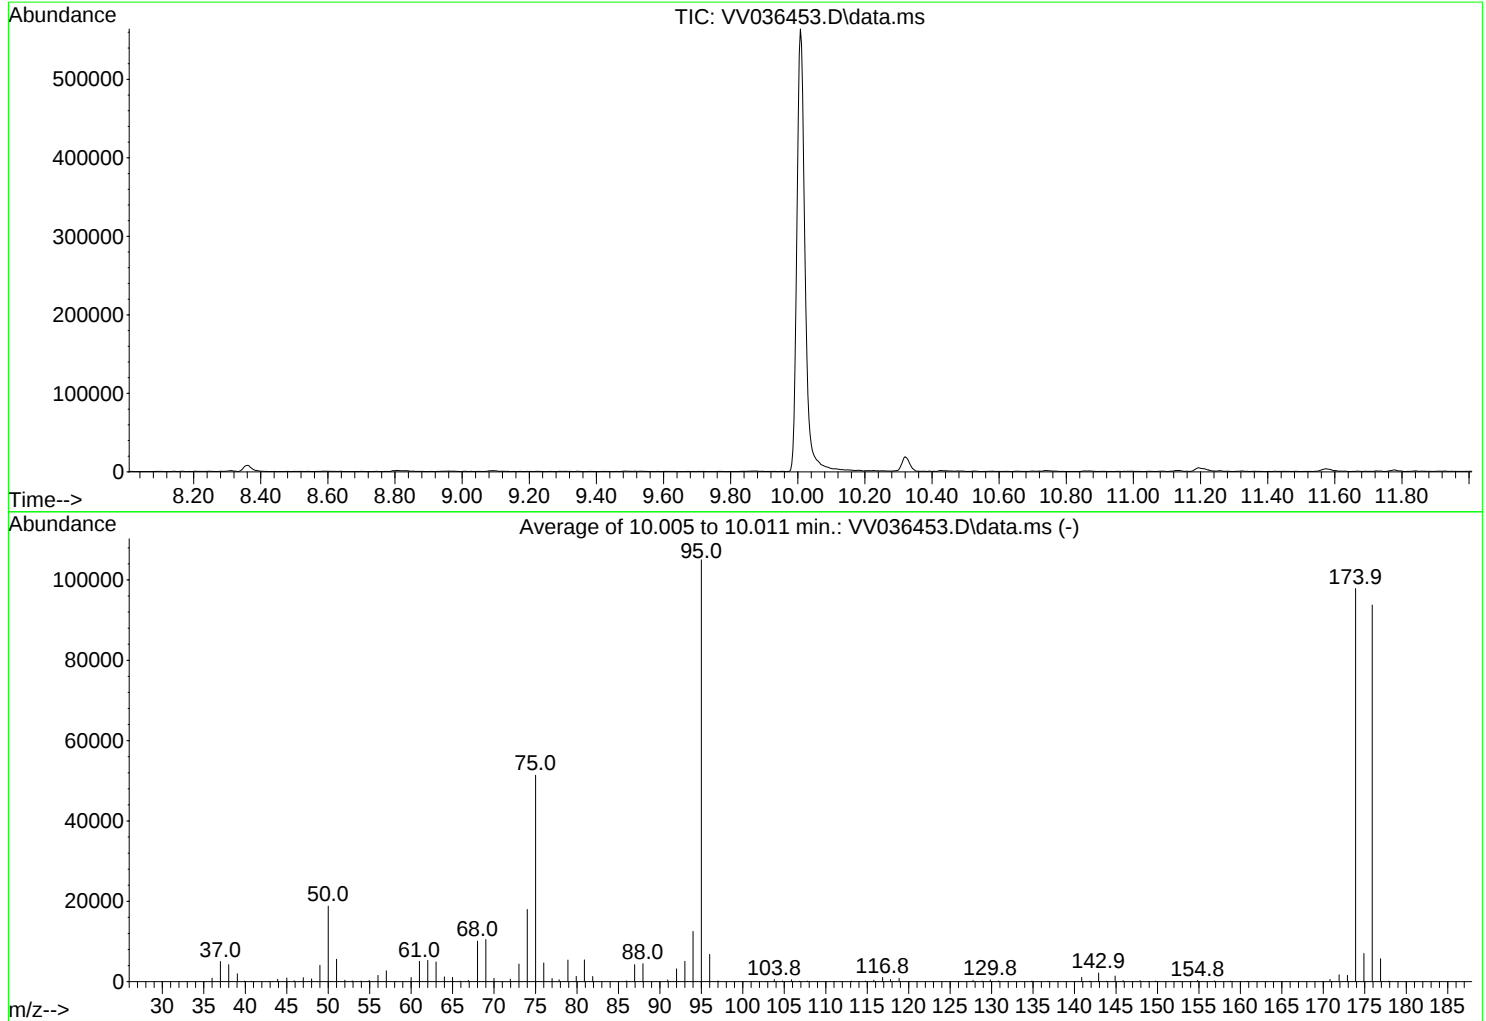

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	18800	PASS
75	95	30	80	48.9	51397	PASS
95	95	100	100	100.0	105003	PASS
96	95	5	9	6.4	6760	PASS
173	174	0.00	2	1.6	1543	PASS
174	95	50	120	93.2	97861	PASS
175	174	5	9	7.2	7026	PASS
176	174	95	101	95.8	93763	PASS
177	176	5	9	6.1	5712	PASS

m/z	Abundance
39.90	119.0
43.80	309.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
36.00	902.0
37.00	5008.0
38.00	4201.0
39.10	1924.0
40.00	259.0
41.00	108.0
42.80	124.0
44.00	904.0
45.00	896.0
45.90	226.0
47.00	1049.0
48.00	700.0
49.00	3952.0
50.00	18792.0
51.00	5573.0
52.00	366.0
52.90	184.0
53.90	147.0
54.90	311.0
56.00	1490.0
57.00	2597.0
60.00	1083.0
61.00	4967.0
62.00	5308.0
63.00	4965.0
64.00	1256.0
65.00	1062.0
65.90	131.0
66.90	325.0
68.00	9845.0
69.00	10304.0
70.00	883.0
72.00	650.0
73.00	4430.0
74.00	18016.0
75.00	51032.0
76.00	4388.0
77.00	730.0
77.90	485.0
78.90	5444.0
79.90	1349.0
80.90	5528.0
81.90	1190.0
85.90	232.0
86.90	4130.0
87.90	4324.0
90.90	461.0
92.00	3238.0
93.00	4959.0
94.00	12482.0
95.00	102096.0
96.00	6725.0
97.00	198.0
103.80	433.0
104.80	198.0
105.90	472.0
106.80	114.0
107.80	139.0
111.80	114.0
113.10	112.0
114.80	142.0
115.80	408.0
116.80	1089.0
117.80	566.0
118.80	774.0
127.70	369.0
128.80	156.0
129.80	453.0
130.90	233.0
134.90	189.0
136.80	129.0
140.90	985.0
141.80	114.0
142.90	2088.0
143.80	147.0
144.90	1282.0
145.90	260.0
147.90	269.0
149.80	176.0
152.70	110.0
154.90	311.0
156.90	194.0
170.80	544.0
171.90	1593.0
172.90	1607.0
173.90	93104.0
174.90	7004.0
175.90	89640.0
176.90	5584.0
177.90	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
36.00	921.0
37.00	5250.0
38.00	4389.0
39.00	1959.0
39.90	311.0
40.70	149.0
44.00	928.0
45.00	940.0
45.90	254.0
47.00	1046.0
48.00	692.0
49.00	4182.0
50.00	19480.0
51.00	5725.0
52.00	364.0
52.90	224.0
53.90	165.0
54.90	308.0
56.00	1609.0
57.00	2769.0
60.00	1045.0
61.00	5223.0
62.00	5522.0
63.00	5011.0
64.00	1241.0
65.00	1097.0
65.90	157.0
66.90	315.0
68.00	10466.0
69.00	10820.0
70.00	902.0
71.90	646.0
73.00	4462.0
74.00	18552.0
75.00	53056.0
76.00	4784.0
77.00	803.0
77.90	490.0
78.90	5545.0
79.90	1372.0
80.90	5527.0
81.90	1299.0
83.00	110.0
85.90	211.0
87.00	4357.0
87.90	4555.0
90.90	442.0
92.00	3288.0
93.00	5229.0
94.00	12929.0
95.00	108112.0
96.00	7018.0
97.00	199.0
102.80	106.0
103.80	506.0
104.80	196.0
105.80	482.0
106.90	127.0
107.80	171.0
111.10	111.0
113.10	132.0
114.80	147.0
115.80	443.0
116.80	1121.0
117.80	537.0
118.90	854.0
127.80	386.0
128.90	147.0
129.80	447.0
130.80	202.0
134.90	179.0
136.80	131.0
140.90	1034.0
141.90	124.0
142.90	2233.0
143.90	135.0
144.90	1466.0
145.90	289.0
147.90	278.0
149.80	175.0
152.80	107.0
154.80	323.0
156.90	230.0
158.80	153.0
160.90	128.0
170.80	594.0
171.90	1759.0
172.90	1576.0
173.90	100936.0
174.90	7181.0
175.90	96552.0
176.90	5837.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

177.90

159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
36.00	835.0
37.00	4794.0
38.00	4109.0
39.00	2005.0
39.90	303.0
40.80	152.0
43.30	100.0
44.00	938.0
45.00	866.0
45.90	232.0
47.00	955.0
48.00	617.0
49.00	4052.0
50.00	18128.0
51.00	5472.0
52.00	328.0
52.90	239.0
54.00	189.0
55.00	307.0
56.00	1545.0
57.00	2723.0
58.20	126.0
60.00	1000.0
61.00	4943.0
62.00	5124.0
63.00	4749.0
64.00	1076.0
65.00	1072.0
65.90	173.0
66.90	283.0
68.00	9944.0
69.00	10330.0
70.00	783.0
71.90	591.0
73.00	4216.0
74.00	17344.0
75.00	50104.0
76.00	4796.0
77.00	806.0
77.80	413.0
78.90	5186.0
79.90	1282.0
80.90	5219.0
81.90	1309.0
83.00	102.0
86.00	209.0
87.00	4238.0
88.00	4495.0
91.00	379.0
92.00	3070.0
93.00	4948.0
94.00	12073.0
95.00	104800.0
96.00	6538.0
97.00	191.0
102.80	114.0
103.80	575.0
104.80	186.0
105.80	459.0
106.90	137.0
107.80	169.0
111.00	113.0
113.10	115.0
114.80	168.0
115.80	392.0
116.90	937.0
117.80	461.0
118.90	870.0
127.80	374.0
128.90	132.0
129.90	400.0
130.80	169.0
134.80	163.0
136.80	143.0
140.80	1059.0
141.90	148.0
142.90	2195.0
143.90	123.0
144.90	1435.0
145.80	253.0
147.90	258.0
148.90	103.0
149.80	145.0
154.80	316.0
156.90	222.0
158.80	176.0
160.80	171.0
170.80	594.0
171.90	1793.0
172.90	1445.0
173.90	99544.0
174.90	6893.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

175.9095096.0

176.905716.0

177.90152.0

Instrument :MSVOA_V

ClientSampleId :BFB327