


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070718\
 Data File : VV006551.D
 Acq On : 07 Jul 2018 07:59
 Operator : SY/MD
 Sample : BFB61
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB61

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jul 09 03:00:48 2018

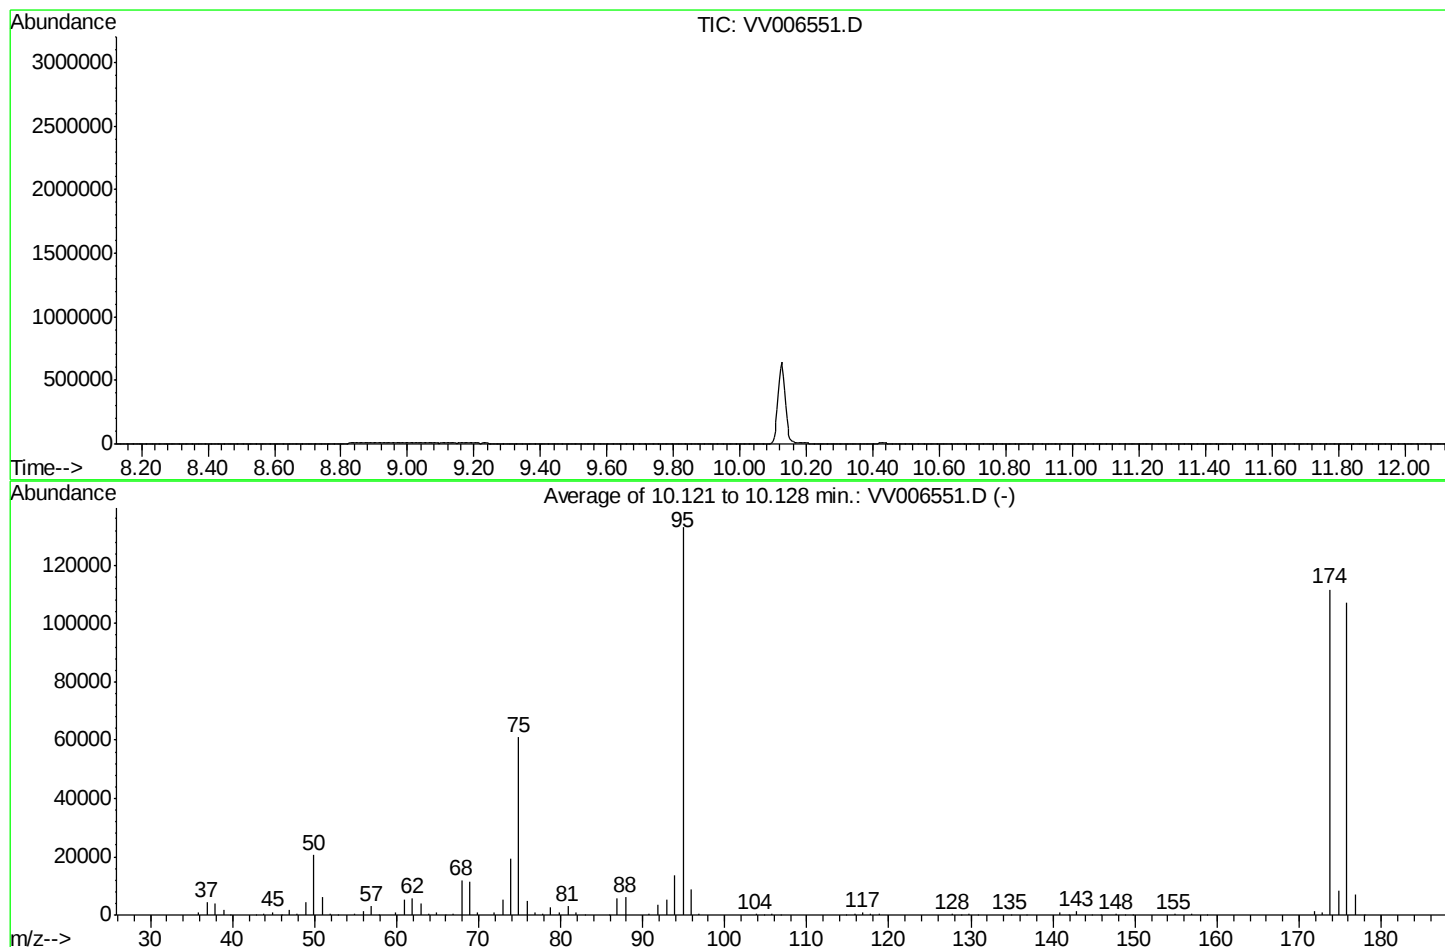

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	20541	PASS
75	95	30	80	45.9	61000	PASS
95	95	100	100	100.0	133042	PASS
96	95	5	9	6.8	8996	PASS
173	174	0.00	2	0.7	837	PASS
174	95	50	120	84.0	111725	PASS
175	174	5	9	7.4	8254	PASS
176	174	95	101	96.1	107362	PASS
177	176	5	9	6.4	6831	PASS

Scan 2858 (10.080 min): VV006551.D
BFB61

m/z	Abundance
35.80	1470.0
36.80	113.0
37.80	520.0
39.80	188.0
43.80	780.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
35.90	2273.0
36.90	4410.0
37.90	4467.0
38.90	1834.0
39.90	274.0
43.80	1164.0
44.90	976.0
46.00	121.0
46.90	1490.0
47.90	607.0
48.90	4211.0
49.90	20408.0
50.90	6273.0
51.90	290.0
52.90	103.0
54.90	334.0
55.90	1416.0
56.90	2828.0
57.90	127.0
59.90	1069.0
60.90	5016.0
61.90	5359.0
62.90	4025.0
63.90	502.0
64.90	1048.0
66.80	306.0
67.90	11530.0
68.90	11556.0
69.90	897.0
71.90	648.0
72.90	5019.0
73.90	18904.0
74.90	59960.0
76.00	4894.0
76.90	820.0
77.80	486.0
78.80	2709.0
79.90	1076.0
80.90	2844.0
81.80	686.0
85.90	217.0
86.90	5564.0
87.90	5804.0
90.80	407.0
91.90	3158.0
92.90	5281.0
93.90	13436.0
94.90	130008.0
95.90	8962.0
96.90	260.0
103.80	403.0
104.80	175.0
105.70	400.0
106.80	152.0
114.80	120.0
115.80	401.0
116.80	794.0
117.80	350.0
118.80	572.0
127.80	407.0
128.80	198.0
129.80	373.0
130.90	135.0
134.90	195.0
136.80	147.0
140.80	990.0
141.90	164.0
142.90	1095.0
144.80	182.0
145.80	185.0
147.70	275.0
148.80	107.0
149.70	127.0
154.80	261.0
156.90	238.0
158.70	123.0
171.80	1276.0
172.80	764.0
173.80	106192.0
174.90	7803.0
175.80	101848.0
176.90	6586.0
177.90	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
35.90	2289.0
36.90	4592.0
37.90	4753.0
38.90	1877.0
39.90	229.0
43.90	1184.0
44.90	964.0
46.00	119.0
46.90	1627.0
47.90	656.0
48.90	4315.0
49.90	21264.0
50.90	6573.0
52.00	286.0
52.90	107.0
54.90	366.0
55.90	1485.0
56.90	3012.0
57.90	134.0
59.90	1091.0
60.90	5283.0
61.90	5719.0
62.90	4151.0
63.90	550.0
64.90	1146.0
65.90	108.0
66.80	316.0
67.90	12294.0
68.90	12013.0
69.90	903.0
71.90	705.0
72.90	5424.0
73.90	19912.0
74.90	63168.0
76.00	5131.0
76.90	898.0
77.70	503.0
78.80	2902.0
79.90	1053.0
80.90	2963.0
81.80	773.0
82.90	110.0
85.90	214.0
86.90	5932.0
87.90	6260.0
90.80	430.0
91.90	3413.0
92.90	5495.0
93.90	14209.0
94.90	137792.0
95.90	9310.0
96.90	264.0
103.80	415.0
104.80	191.0
105.80	412.0
106.80	150.0
114.70	113.0
115.80	465.0
116.90	844.0
117.80	369.0
118.80	626.0
127.80	449.0
128.80	221.0
129.80	437.0
130.90	127.0
134.80	197.0
136.80	164.0
140.80	1086.0
141.80	158.0
142.90	1236.0
144.80	215.0
145.80	211.0
147.70	289.0
148.80	109.0
149.70	148.0
154.90	271.0
156.90	269.0
158.80	112.0
171.80	1454.0
172.80	842.0
173.80	115504.0
174.90	8549.0
175.80	110800.0
176.90	7091.0
178.00	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
35.90	2167.0
36.90	4267.0
37.90	4543.0
38.90	1849.0
39.80	194.0
42.80	108.0
43.90	1209.0
44.90	881.0
46.00	132.0
46.90	1572.0
47.90	632.0
48.90	4050.0
49.90	19952.0
50.90	6269.0
52.00	249.0
52.80	101.0
54.90	332.0
55.90	1451.0
56.90	2893.0
57.90	115.0
59.90	1061.0
60.90	5045.0
61.90	5577.0
62.90	3839.0
63.90	555.0
64.90	1090.0
65.90	140.0
66.80	291.0
67.90	11614.0
68.90	11313.0
69.90	803.0
71.90	694.0
72.90	5233.0
73.90	18968.0
74.90	59872.0
76.00	4906.0
76.90	833.0
77.70	531.0
78.80	2874.0
79.90	915.0
80.90	2848.0
81.80	779.0
83.00	138.0
85.90	191.0
86.90	5720.0
87.90	6100.0
90.80	410.0
91.90	3388.0
92.90	5200.0
93.90	13689.0
94.90	131328.0
95.90	8717.0
96.90	256.0
103.80	400.0
104.80	176.0
105.80	395.0
106.80	120.0
115.80	457.0
116.90	799.0
117.80	380.0
118.80	600.0
127.80	445.0
128.80	251.0
129.80	420.0
130.90	116.0
134.80	193.0
136.80	165.0
140.80	1067.0
141.80	127.0
142.90	1221.0
144.70	213.0
145.70	217.0
147.80	308.0
149.70	143.0
154.90	268.0
156.80	237.0
171.80	1436.0
172.90	905.0
173.80	113480.0
174.90	8410.0
175.80	109440.0
176.90	6818.0
178.00	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61