

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070824\Not Reviewed data\
 Data File : VV036466.D
 Acq On : 08 Jul 2024 13:13
 Operator : SY/MD
 Sample : P3101-06
 Misc : 5.00g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 09 15:38:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 09 00:54:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	265186	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	288805	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	139145	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	103975	23.087	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.360%
7) Chloroethane-d5	1.529	69	84426	23.470	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.880%
11) 1,1-Dichloroethene-d2	2.050	65	48991	23.140	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	92.560%
21) 2-Butanone-d5	3.834	46	24469	23.410	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	46.820%
24) Chloroform-d	4.246	84	173316	22.141	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.560%
26) 1,2-Dichloroethane-d4	4.941	65	93605	22.424	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.680%
32) Benzene-d6	4.957	84	327181	20.069	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.280%
36) 1,2-Dichloropropane-d6	5.986	67	100510	20.496	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.000%
41) Toluene-d8	7.243	98	279328	19.003	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.000%
43) trans-1,3-Dichloroprop...	7.555	79	41067	18.753	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.000%
47) 2-Hexanone-d5	8.034	63	20935	26.745	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	53.480%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	80224	19.958	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.840%
66) 1,2-Dichlorobenzene-d4	11.558	152	111825	22.053	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.200%
Target Compounds						
					Qvalue	
10) 1,1,2-Trichloro-1,2,2-...	2.050	101	1849	0.392	ug/L #	28
25) Chloroform	4.278	83	5046	0.642	ug/L	88
48) 2-Hexanone	8.034	43	2612	1.348	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070824\Not Reviewed data\
Data File : VV036466.D
Acq On : 08 Jul 2024 13:13
Operator : SY/MD
Sample : P3101-06
Misc : 5.00g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jul 09 15:38:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 09 00:54:05 2024
Response via : Initial Calibration

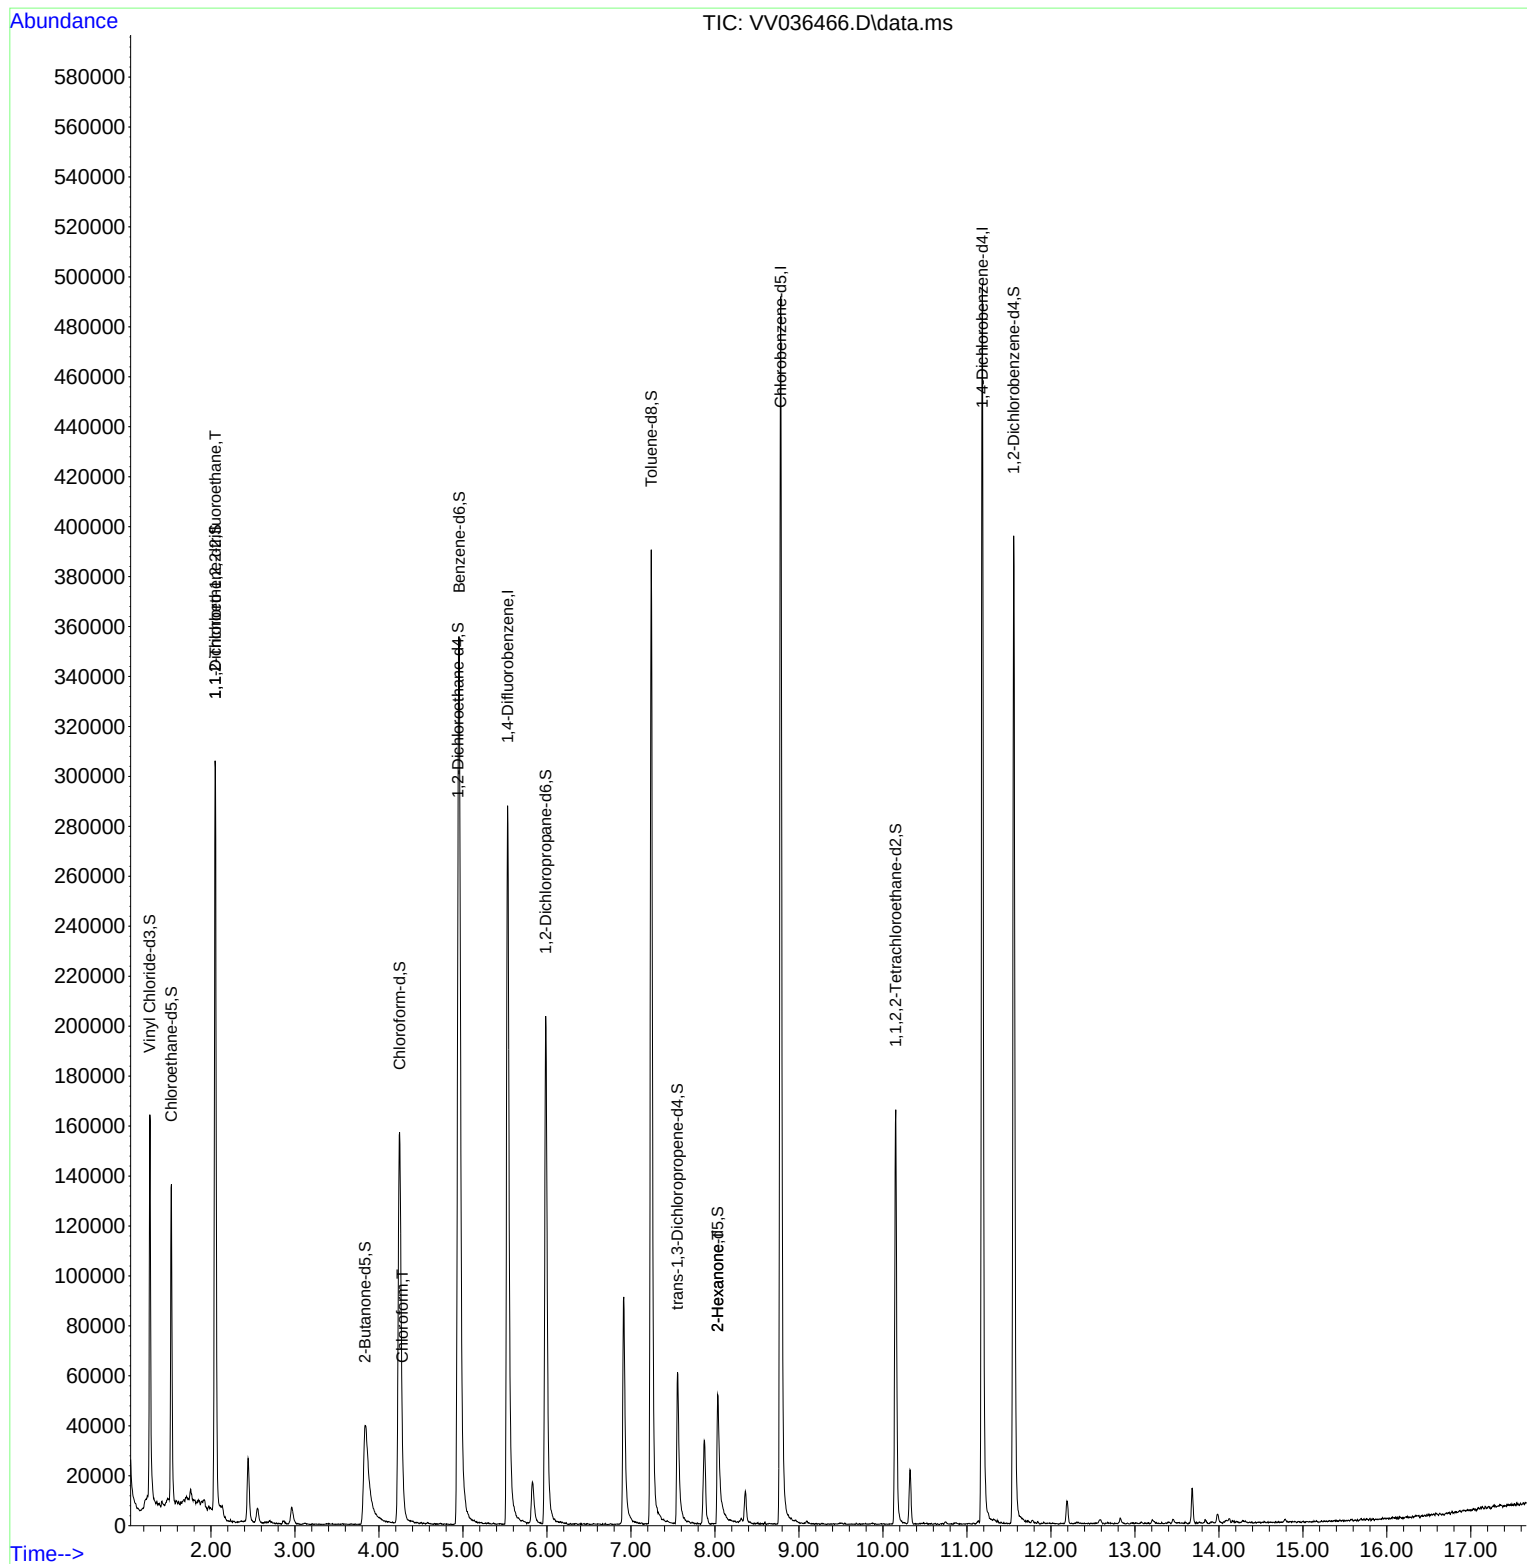



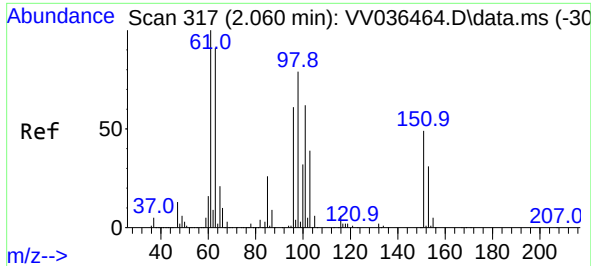


#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.392 ug/L
RT: 2.050 min Scan# 317
Delta R.T. -0.010 min
Lab File: VV036466.D
Acq: 08 Jul 2024 13:13

Instrument :
MSVOA_V
ClientSampleId :



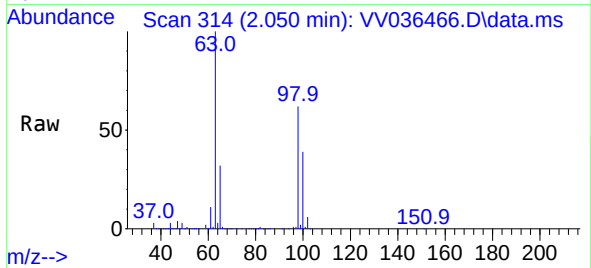



Tgt Ion:101 Resp: 1849
Ion Ratio Lower Upper
101 100
85 6.5 34.6 51.8#
151 6.3 58.9 88.3#

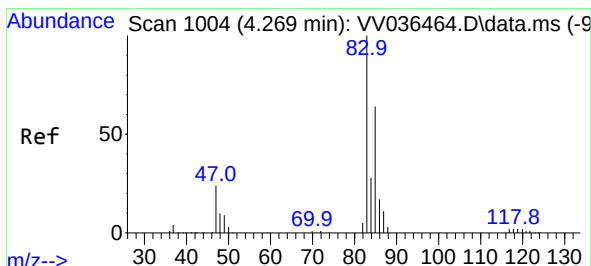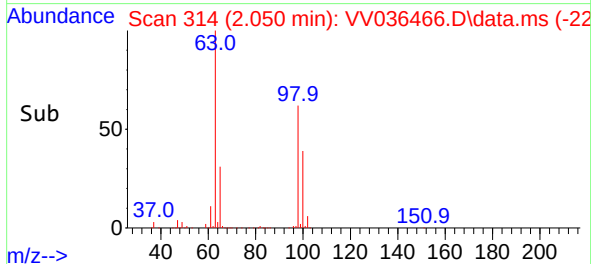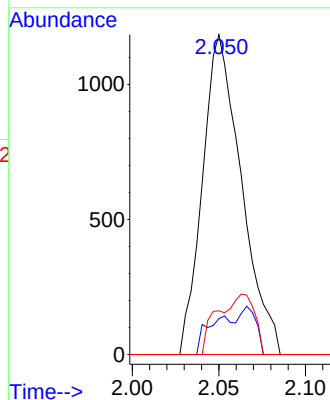

#25
Chloroform
Concen: 0.642 ug/L
RT: 4.278 min Scan# 1007
Delta R.T. 0.010 min
Lab File: VV036466.D
Acq: 08 Jul 2024 13:13


Tgt Ion: 83 Resp: 5046
Ion Ratio Lower Upper
83 100
85 73.5 45.0 83.6

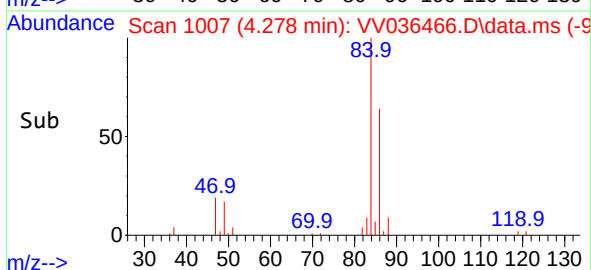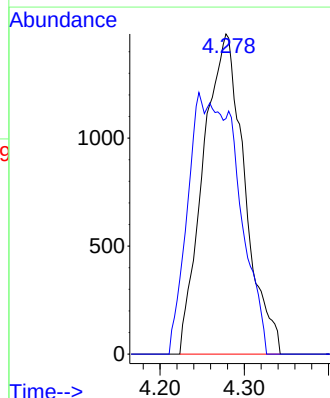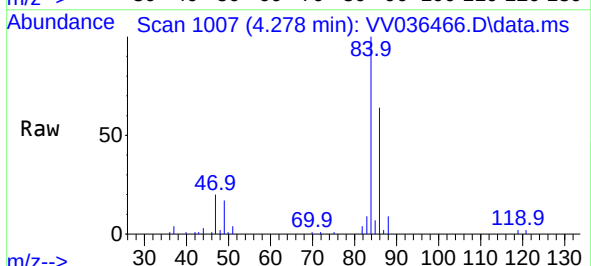

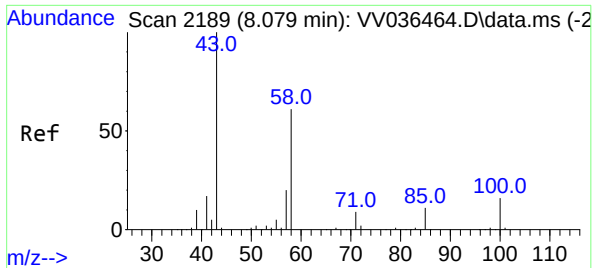

#48
2-Hexanone
Concen: 1.348 ug/L
RT: 8.034 min Scan# 21
Delta R.T. -0.045 min
Lab File: VV036466.D
Acq: 08 Jul 2024 13:13

Instrument :
MSVOA_V
ClientSampleId :

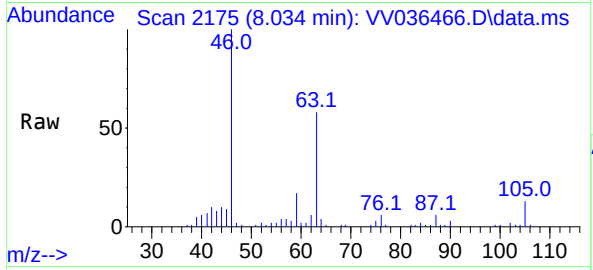

Tgt Ion: 43	Resp: 2612
Ion Ratio	Lower Upper
43 100	
58 40.0	48.5 72.7#
57 49.3	15.8 23.6#
100 5.0	10.9 16.3#

