

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
 Data File : VV026718.D
 Acq On : 12 Jul 2022 11:41
 Operator : SY/MD
 Sample : VV0712WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK392

Quant Time: Jul 13 03:00:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 13 02:57:58 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.613	114	214298	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.850	117	217531	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.246	152	85347	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.301	65	104270	5.333	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.600%	
7) Chloroethane-d5		1.558	69	94042	5.567	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.400%	
11) 1,1-Dichloroethene-d2		2.098	63	151426	4.035	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.600%	
20) 2-Butanone-d5		3.925	46	165042	54.090	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.180%	
24) Chloroform-d		4.339	84	181527	5.310	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.200%	
26) 1,2-Dichloroethane-d4		5.031	65	84500	5.658	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.200%	
32) Benzene-d6		5.040	84	327390	4.953	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%	
36) 1,2-Dichloropropane-d6		6.069	67	106299	5.364	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.200%	
41) Toluene-d8		7.313	98	251952	4.294	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.800%	
43) trans-1,3-Dichloroprop...		7.622	79	30697	4.734	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.600%	
46) 2-Hexanone-d5		8.095	63	125402	44.669	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.340%	
56) 1,1,2,2-Tetrachloroeth...		10.214	84	76544	4.958	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.200%	
66) 1,2-Dichlorobenzene-d4		11.622	152	80140	5.389	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.800%	
Target Compounds							Qvalue
16) Methylene chloride		2.500	84	4777	0.213	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026718.D
Acq On : 12 Jul 2022 11:41
Operator : SY/MD
Sample : VV0712WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK392

Quant Time: Jul 13 03:00:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 13 02:57:58 2022
Response via : Initial Calibration

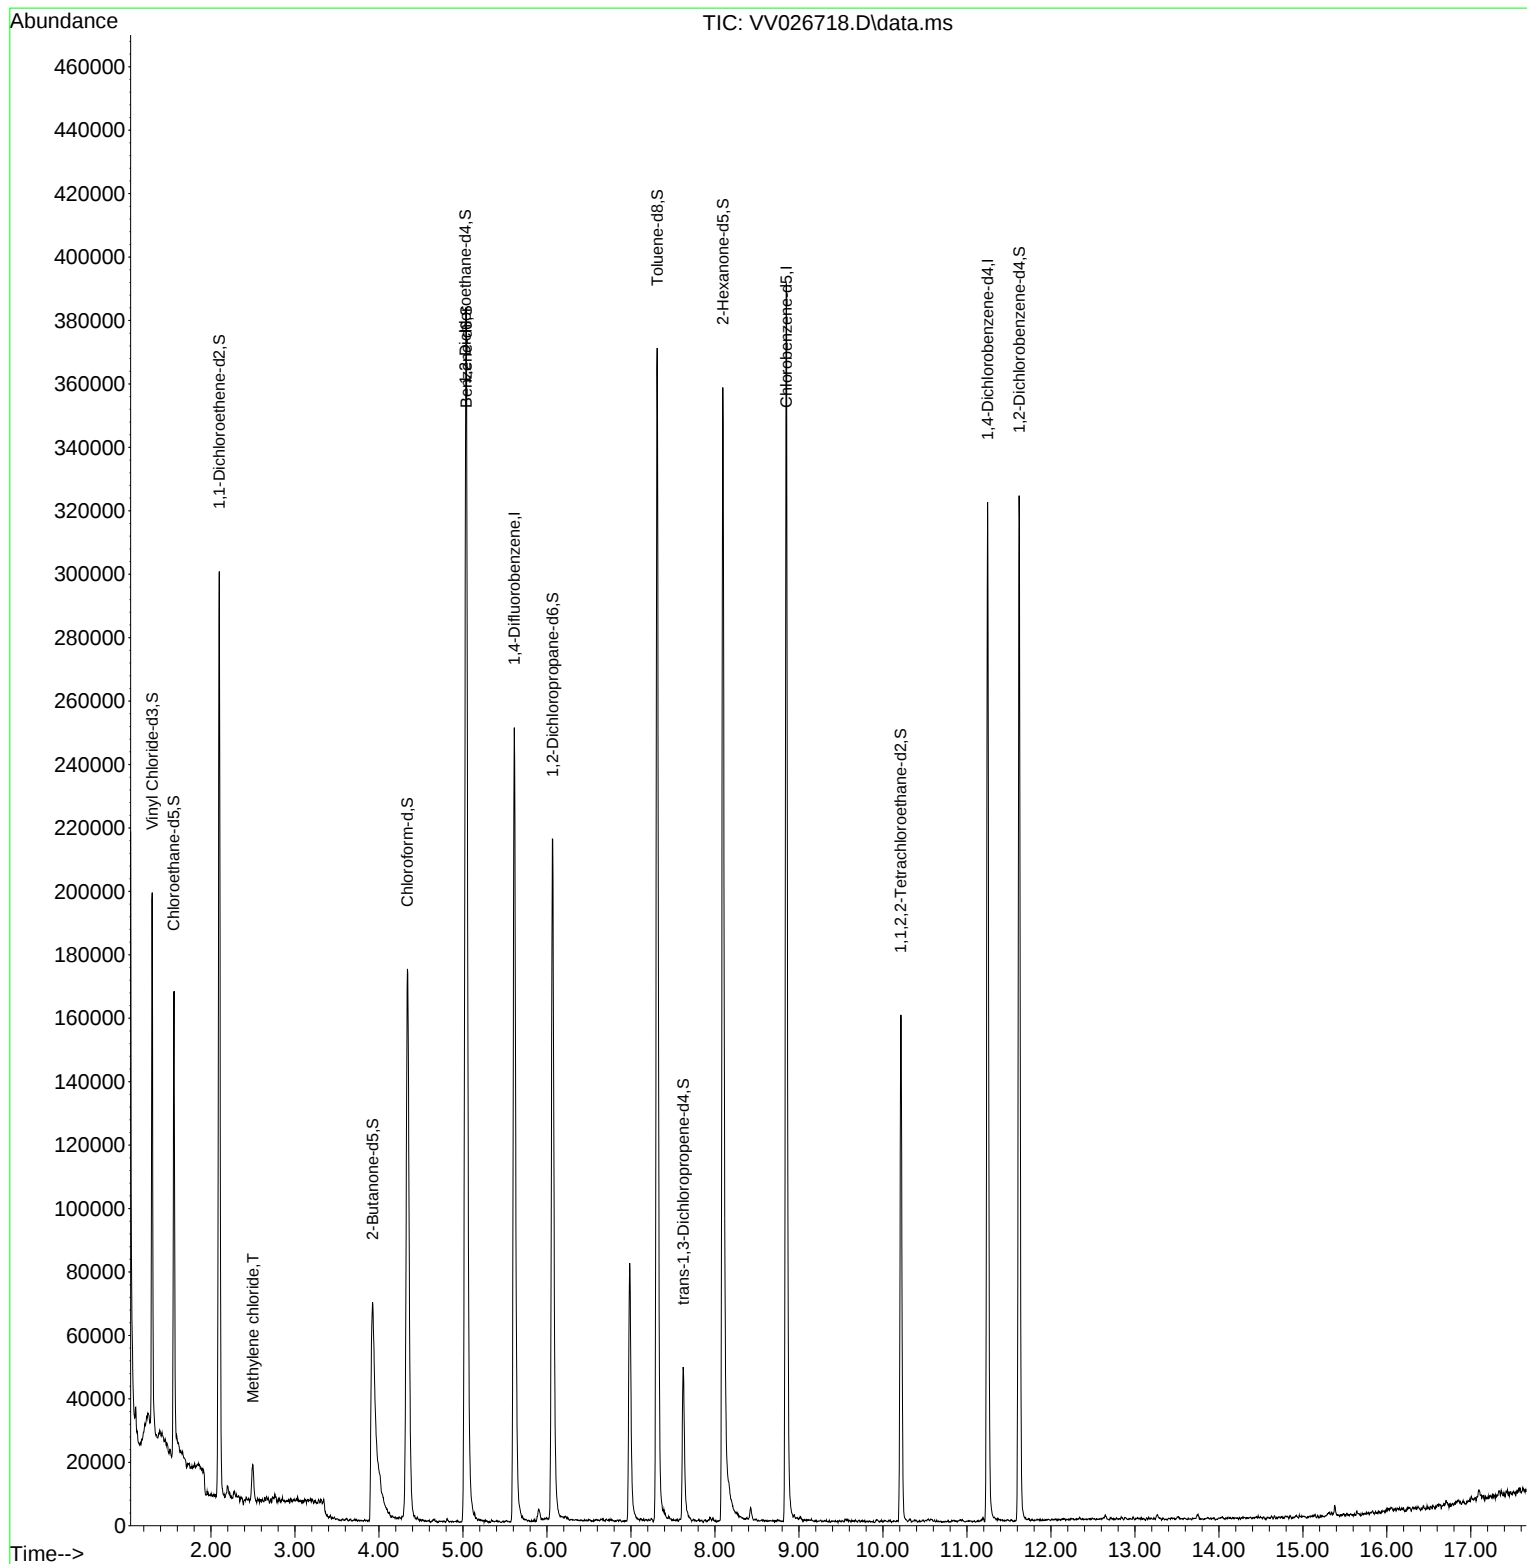

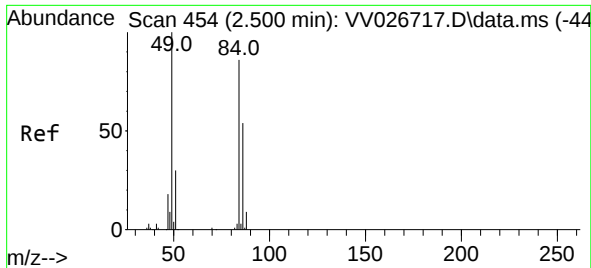

#16
Methylene chloride
Concen: 0.213 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV026718.D
Acq: 12 Jul 2022 11:41

Instrument :
MSVOA_V
ClientSampleId :
VBLK392

Tgt Ion: 84 Resp: 4777

Ion	Ratio	Lower	Upper
84	100		
86	62.4	44.8	83.2
49	107.5	78.7	146.1

