

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071222\
 Data File : VW026721.D
 Acq On : 12 Jul 2022 12:56
 Operator : SY/MD
 Sample : N3601-14 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC3

Quant Time: Jul 13 03:00:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 13 02:57:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	233786	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	219744	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	84990	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.291	65	103519	4.854	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	97.000%	
7) Chloroethane-d5	1.555	69	91530	4.967	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.400%	
11) 1,1-Dichloroethene-d2	2.095	63	148727	3.632	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.600%	
20) 2-Butanone-d5	3.953	46	256494	77.055	ug/L	0.05
Spiked Amount	50.000	Range 40 - 130	Recovery	=	154.100%#	
24) Chloroform-d	4.336	84	197033	5.283	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	105.600%	
26) 1,2-Dichloroethane-d4	5.024	65	97827	6.005	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	120.000%	
32) Benzene-d6	5.030	84	419593	6.284	ug/L	-0.01
Spiked Amount	5.000	Range 70 - 125	Recovery	=	125.600%#	
36) 1,2-Dichloropropane-d6	6.066	67	105458	5.268	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	105.400%	
41) Toluene-d8	7.310	98	245073	4.135	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.600%	
43) trans-1,3-Dichloroprop...	7.622	79	28949	4.420	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.400%	
46) 2-Hexanone-d5	8.104	63	134893	47.566	ug/L	0.02
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.140%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	76714	4.919	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	79842	5.392	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.497	84	10314	0.422	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026721.D
Acq On : 12 Jul 2022 12:56
Operator : SY/MD
Sample : N3601-14 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC3

Quant Time: Jul 13 03:00:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 13 02:57:58 2022
Response via : Initial Calibration

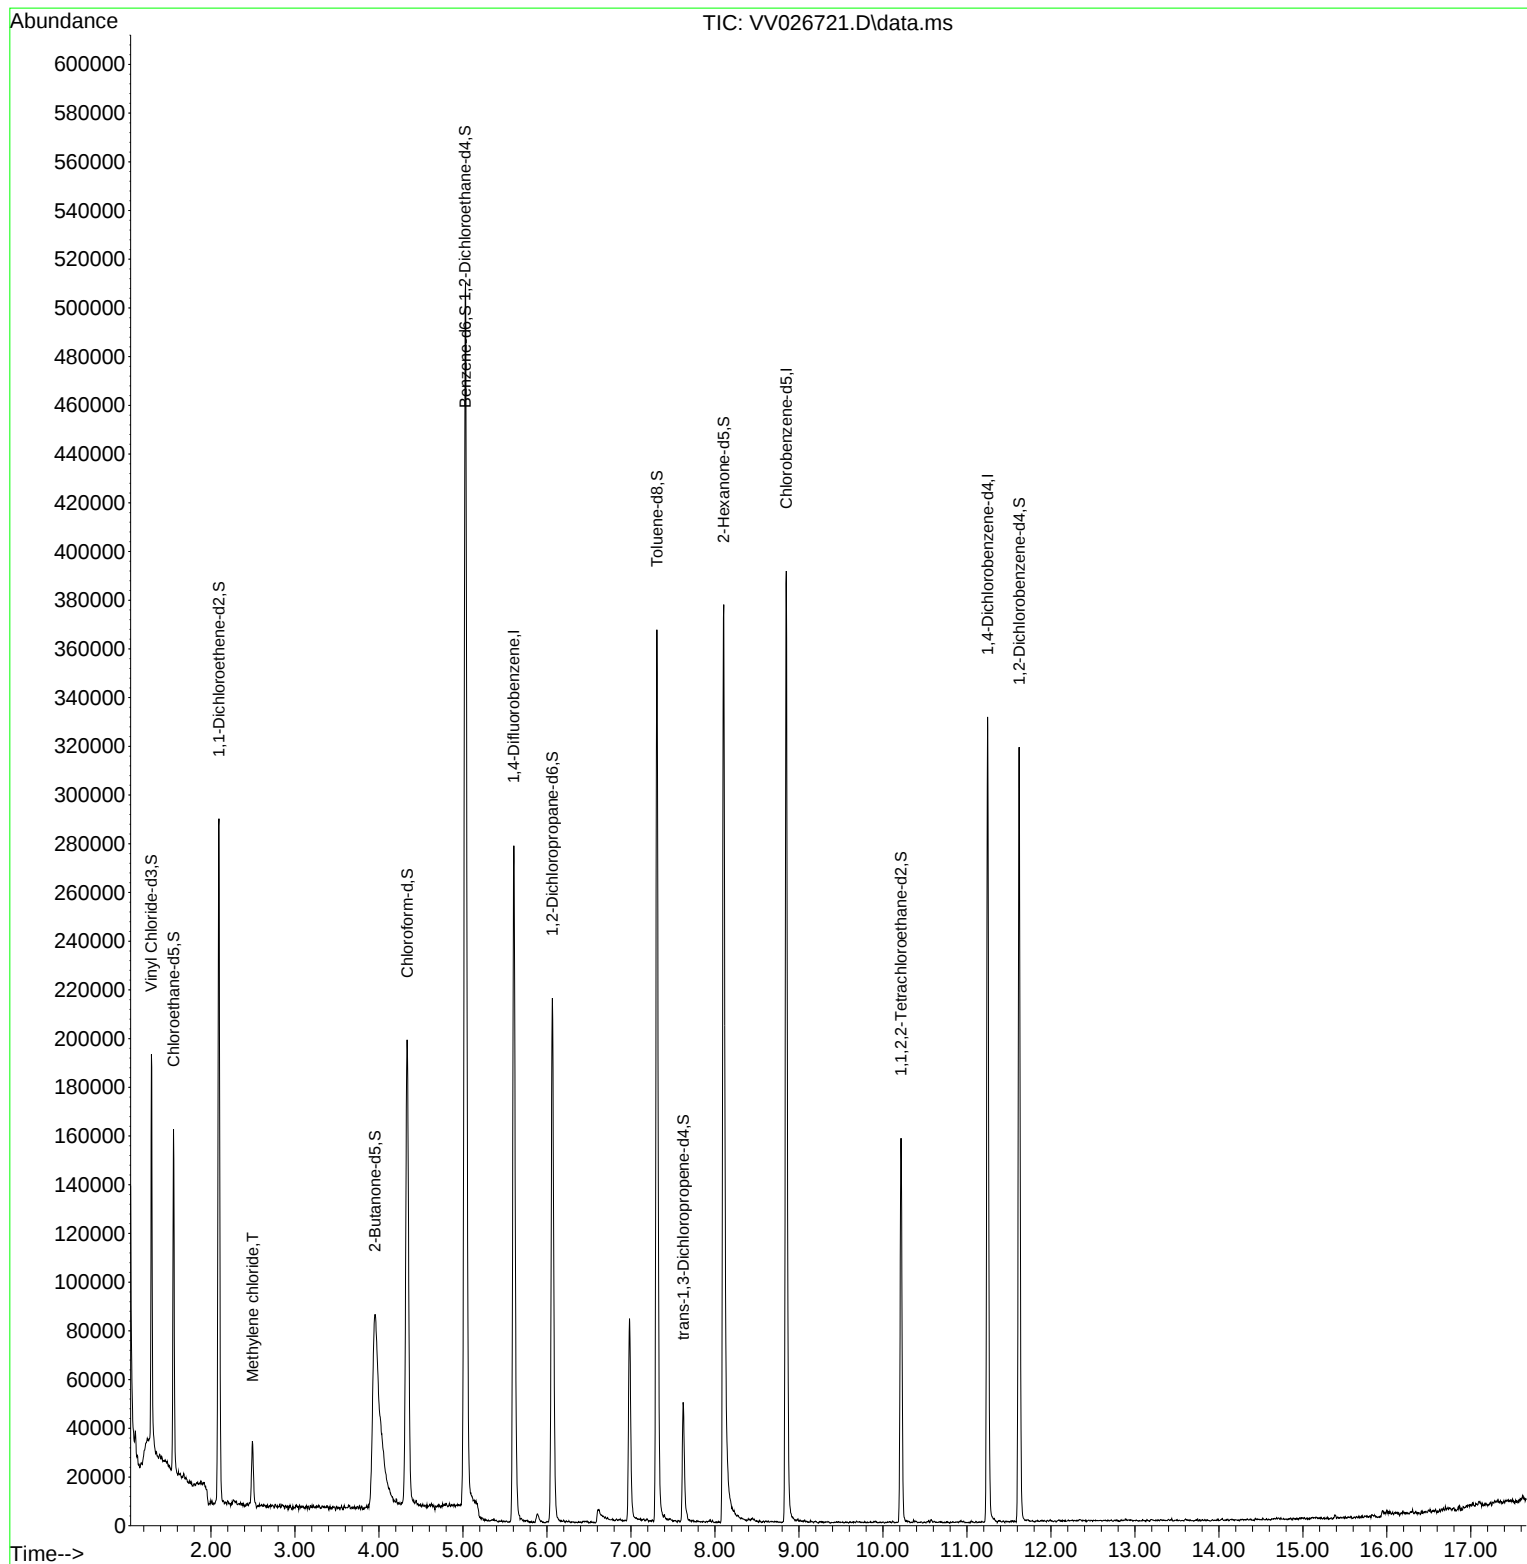

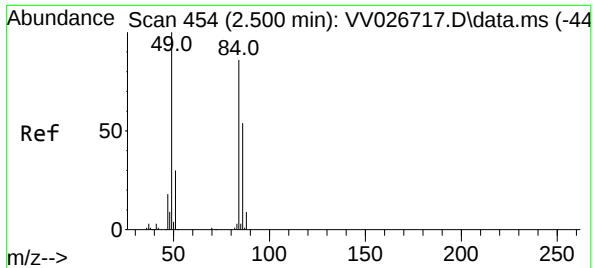

#16
Methylene chloride
Concen: 0.422 ug/L
RT: 2.497 min Scan# 41
Delta R.T. -0.003 min
Lab File: VV026721.D
Acq: 12 Jul 2022 12:56

Instrument :
MSVOA_V
ClientSampleId :
DBUC3

Tgt Ion: 84 Resp: 10314
Ion Ratio Lower Upper
84 100
86 69.6 44.8 83.2
49 125.1 78.7 146.1

