

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
 Data File : VV026719.D
 Acq On : 12 Jul 2022 12:06
 Operator : SY/MD
 Sample : N3601-11 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUB8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026719.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	165518	181700	19.87%	2.588%
2	1.561	155	162	173	rVB	143862	161418	17.65%	2.299%
3	2.098	319	329	353	rVB	284734	413448	45.20%	5.889%
4	2.500	443	454	468	rVB2	27010	44379	4.85%	0.632%
5	3.908	879	892	925	rBV	65365	261968	28.64%	3.732%
6	4.342	1011	1027	1053	rBV	168417	424594	46.42%	6.048%
7	5.043	1228	1245	1281	rBV2	368750	914630	100.00%	13.028%
8	5.613	1410	1422	1448	rBV	251199	527531	57.68%	7.514%
9	5.912	1505	1515	1529	rBV10	4315	9299	1.02%	0.132%
10	6.066	1547	1563	1583	rBV	215080	446867	48.86%	6.365%
11	6.985	1838	1849	1876	rBV2	79910	157123	17.18%	2.238%
12	7.313	1939	1951	1976	rBV	379901	669003	73.14%	9.530%
13	7.622	2036	2047	2066	rBV	48852	93833	10.26%	1.337%
14	8.088	2181	2192	2236	rBV	340554	721230	78.85%	10.274%
15	8.850	2414	2429	2456	rBV	400313	664186	72.62%	9.461%
16	10.214	2842	2853	2872	rBV	160280	255031	27.88%	3.633%
17	11.246	3163	3174	3190	rBV	332685	519426	56.79%	7.399%
18	11.622	3280	3291	3308	rBV	331650	522451	57.12%	7.442%
19	15.924	4612	4629	4630	rBV	16898	32128	3.51%	0.458%




Sum of corrected areas: 7020245

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026719.D
Acq On : 12 Jul 2022 12:06
Operator : SY/MD
Sample : N3601-11 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

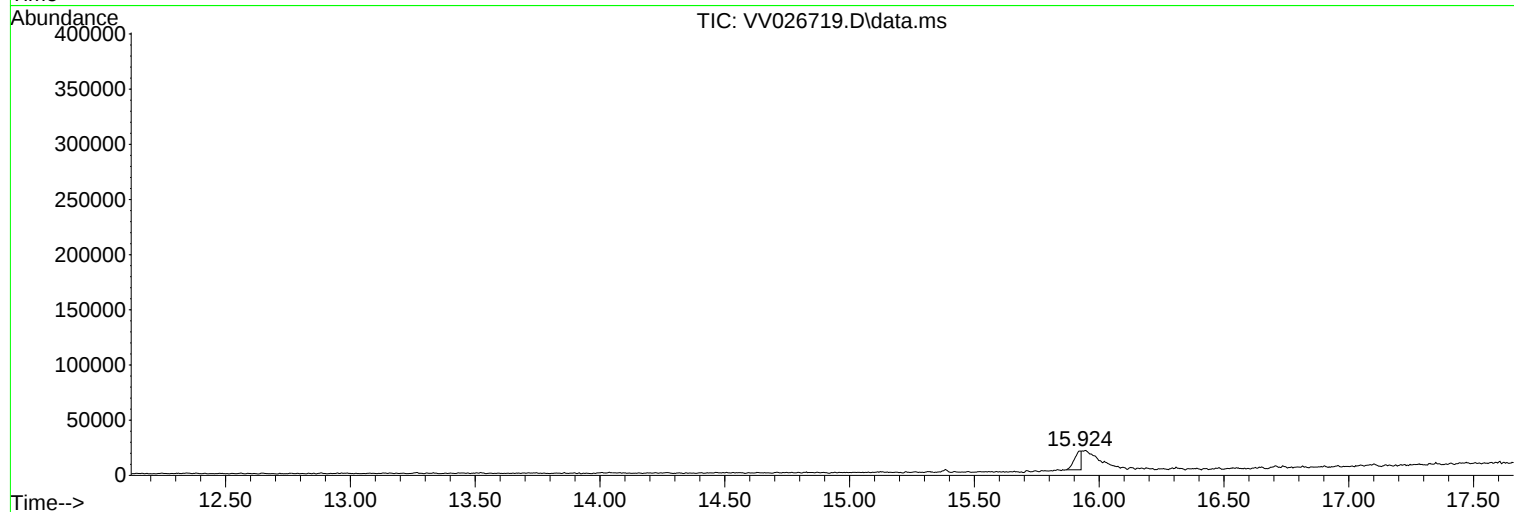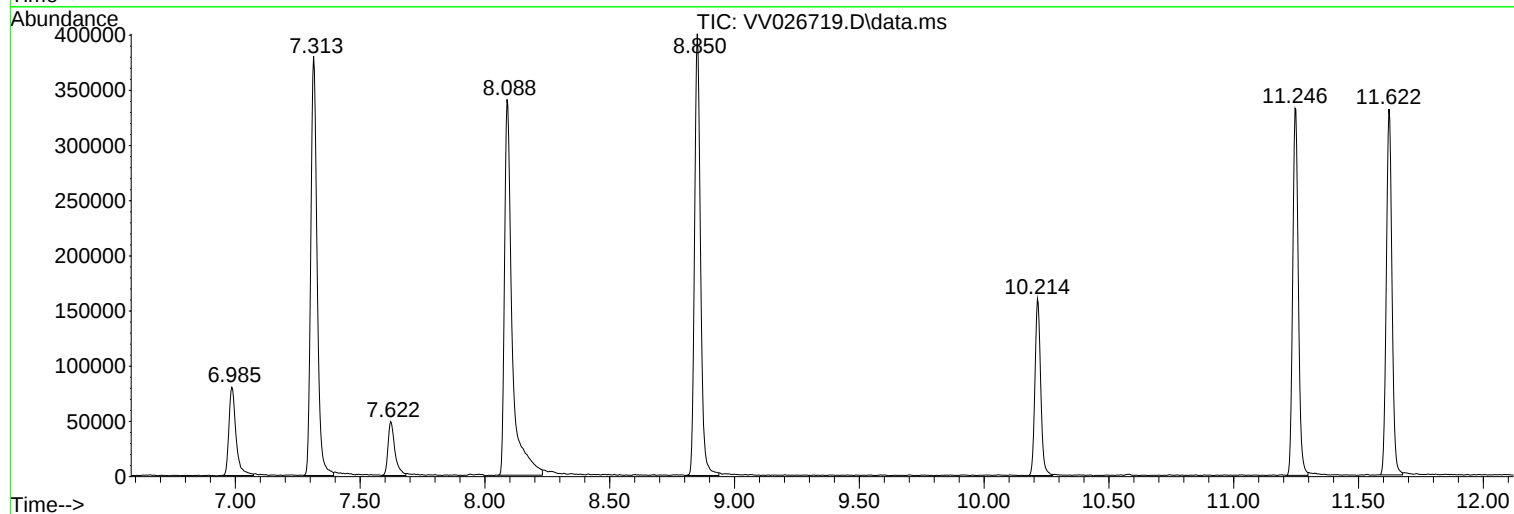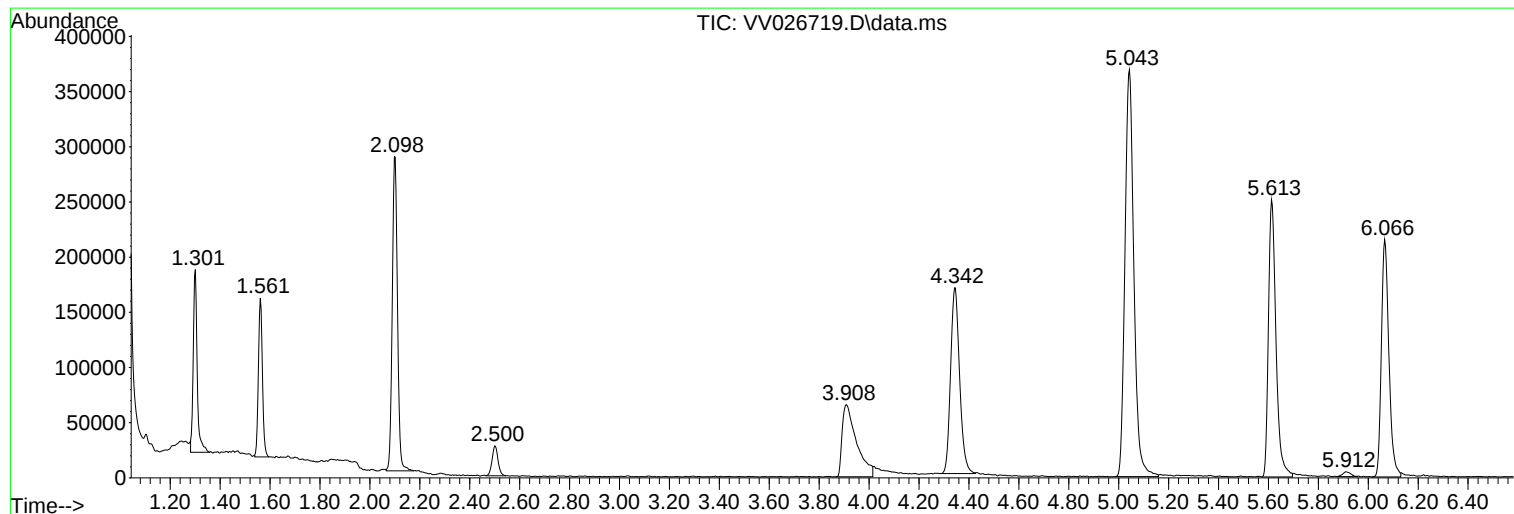

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026719.D
Acq On : 12 Jul 2022 12:06
Operator : SY/MD
Sample : N3601-11 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026719.D
Acq On : 12 Jul 2022 12:06
Operator : SY/MD
Sample : N3601-11 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc