

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
 Data File : VV026730.D
 Acq On : 12 Jul 2022 17:01
 Operator : SY/MD
 Sample : N3601-20DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUB3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026730.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	74	80	102	rVB	156378	175915	19.84%	2.405%
2	1.561	155	162	176	rVB	129142	145838	16.45%	1.994%
3	2.098	320	329	345	rVB	263677	382601	43.15%	5.231%
4	2.500	443	454	471	rVB2	39035	67175	7.58%	0.918%
5	3.902	877	890	925	rBV3	145532	460437	51.93%	6.295%
6	4.342	1010	1027	1052	rVB2	161724	403124	45.46%	5.512%
7	5.043	1229	1245	1276	rBV2	353983	886672	100.00%	12.123%
8	5.616	1410	1423	1443	rBV2	133479	280143	31.59%	3.830%
9	5.912	1502	1515	1537	rBV	218557	446934	50.41%	6.111%
10	6.066	1548	1563	1596	rBV	205905	437479	49.34%	5.981%
11	6.985	1838	1849	1868	rBV	62631	124615	14.05%	1.704%
12	7.313	1938	1951	1978	rBV	369872	656203	74.01%	8.972%
13	7.625	2036	2048	2062	rBV2	36336	67209	7.58%	0.919%
14	7.973	2136	2156	2174	rBV	394045	669328	75.49%	9.151%
15	8.088	2182	2192	2238	rBV	339065	706875	79.72%	9.664%
16	8.850	2418	2429	2447	rBV	212258	356054	40.16%	4.868%
17	10.214	2841	2853	2870	rBV	151945	245622	27.70%	3.358%
18	11.249	3165	3175	3195	rBV	186760	295093	33.28%	4.035%
19	11.622	3280	3291	3308	rBV	319924	506830	57.16%	6.929%




Sum of corrected areas: 7314147

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026730.D
Acq On : 12 Jul 2022 17:01
Operator : SY/MD
Sample : N3601-20DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

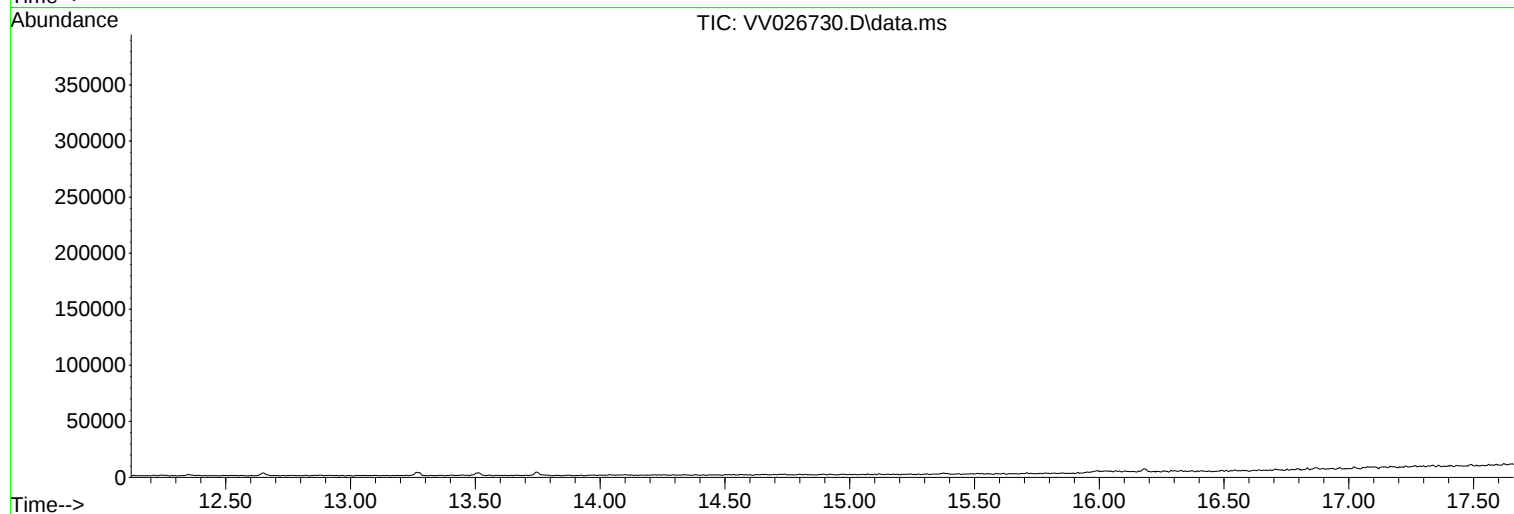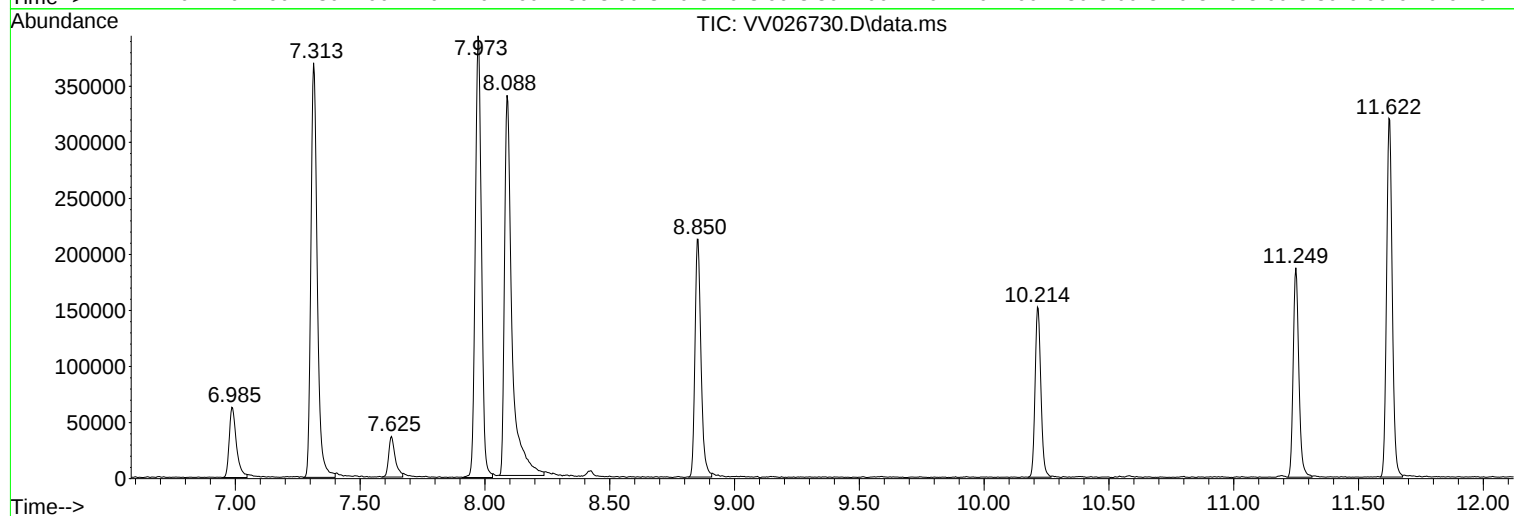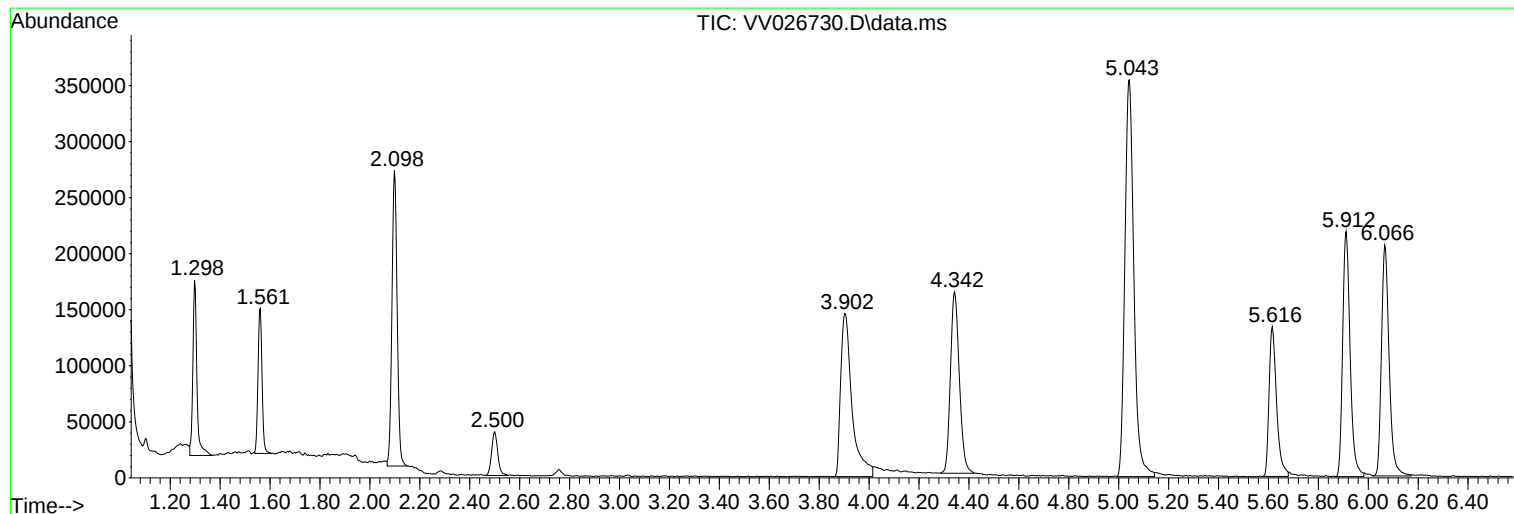

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026730.D
Acq On : 12 Jul 2022 17:01
Operator : SY/MD
Sample : N3601-20DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026730.D
Acq On : 12 Jul 2022 17:01
Operator : SY/MD
Sample : N3601-20DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc