

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
 Data File : VV026731.D
 Acq On : 12 Jul 2022 17:24
 Operator : SY/MD
 Sample : N3601-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUB6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	30	rVB2	15857	15286	2.07%	0.280%
2	1.301	75	81	99	rVB	132500	144596	19.55%	2.648%
3	1.561	156	162	177	rVB	112297	129150	17.46%	2.365%
4	2.101	321	330	349	rVB	228926	345159	46.66%	6.320%
5	3.908	881	892	940	rBV2	53832	259513	35.08%	4.752%
6	4.346	1009	1028	1054	rBV	136412	343639	46.45%	6.293%
7	5.047	1230	1246	1278	rBV2	295106	739802	100.00%	13.547%
8	5.619	1413	1424	1450	rBV	142775	305351	41.27%	5.591%
9	5.921	1506	1518	1536	rBV6	21505	49648	6.71%	0.909%
10	6.069	1551	1564	1593	rBV	172121	364511	49.27%	6.675%
11	6.397	1655	1666	1683	rBV2	7667	18936	2.56%	0.347%
12	6.989	1840	1850	1869	rBV3	55297	107109	14.48%	1.961%
13	7.317	1939	1952	1981	rBV	298185	542776	73.37%	9.939%
14	7.629	2039	2049	2065	rBV2	29612	57170	7.73%	1.047%
15	7.976	2149	2157	2176	rVB2	14581	25412	3.43%	0.465%
16	8.092	2181	2193	2233	rBV	309480	631967	85.42%	11.572%
17	8.854	2417	2430	2452	rBV	230674	394214	53.29%	7.219%
18	10.217	2843	2854	2869	rBV	136303	215679	29.15%	3.949%
19	11.249	3163	3175	3197	rBV	203602	319325	43.16%	5.847%
20	11.535	3255	3264	3276	rBV3	5632	9788	1.32%	0.179%
21	11.625	3280	3292	3308	rBV	276010	441990	59.74%	8.094%




Sum of corrected areas: 5461021

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026731.D
Acq On : 12 Jul 2022 17:24
Operator : SY/MD
Sample : N3601-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

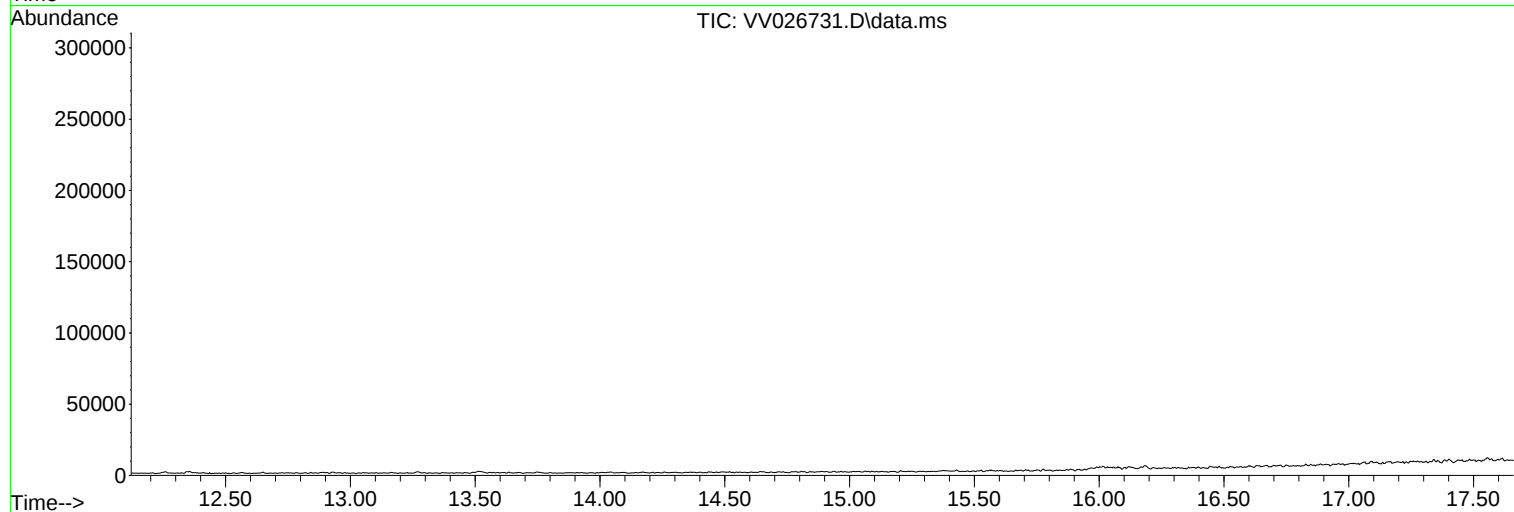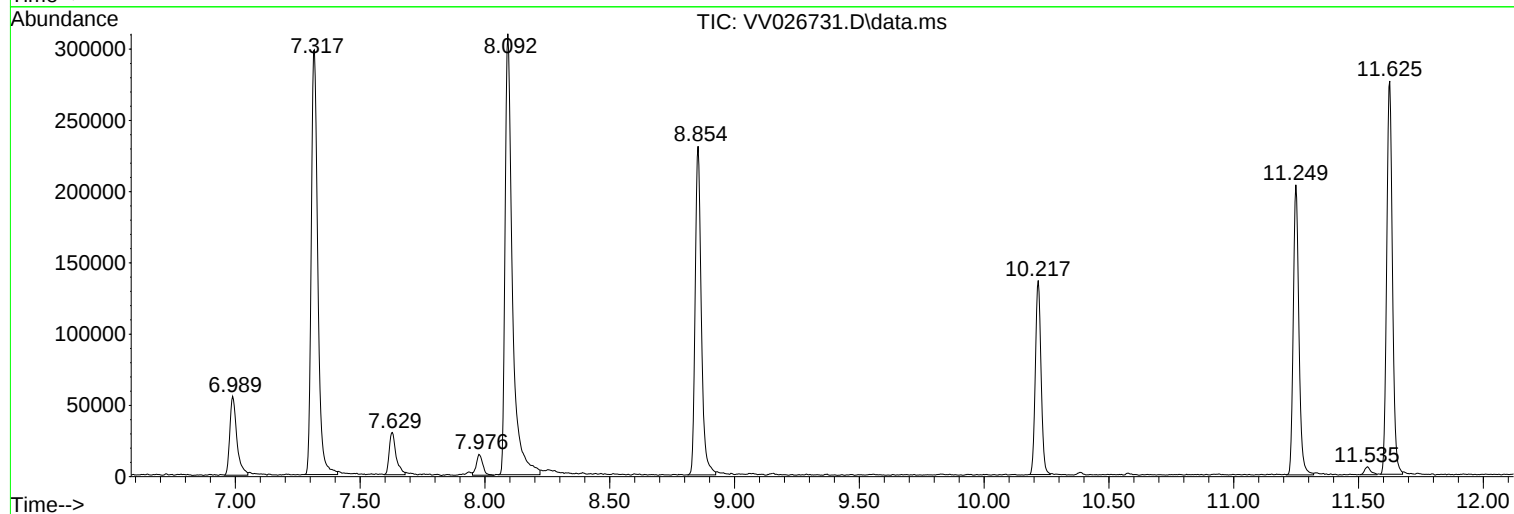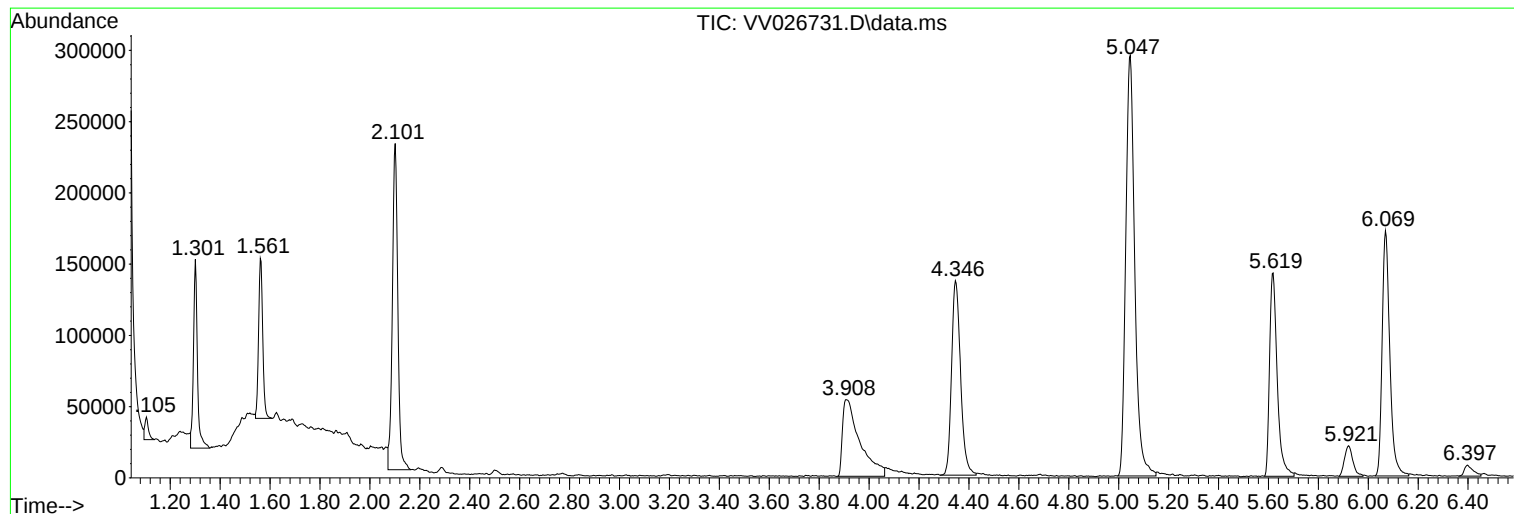

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026731.D
Acq On : 12 Jul 2022 17:24
Operator : SY/MD
Sample : N3601-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026731.D
Acq On : 12 Jul 2022 17:24
Operator : SY/MD
Sample : N3601-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
