
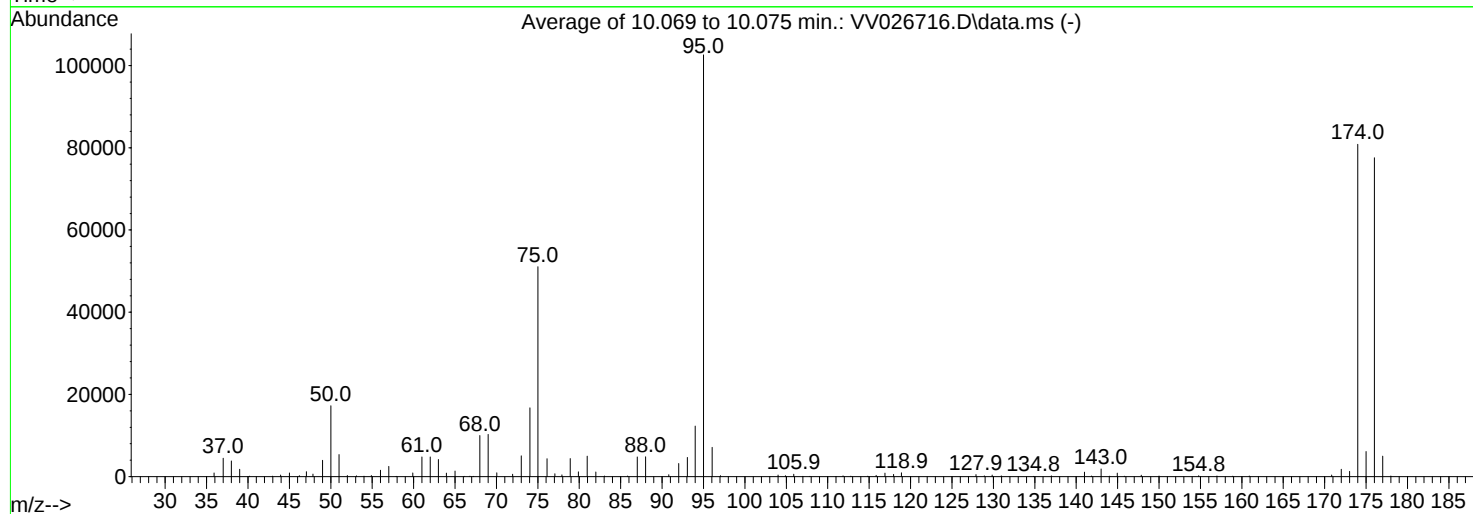


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071222\
Data File : VV026716.D
Acq On : 12 Jul 2022 09:29
Operator : SY/MD
Sample : BFB343
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB343

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Jul 13 02:57:58 2022

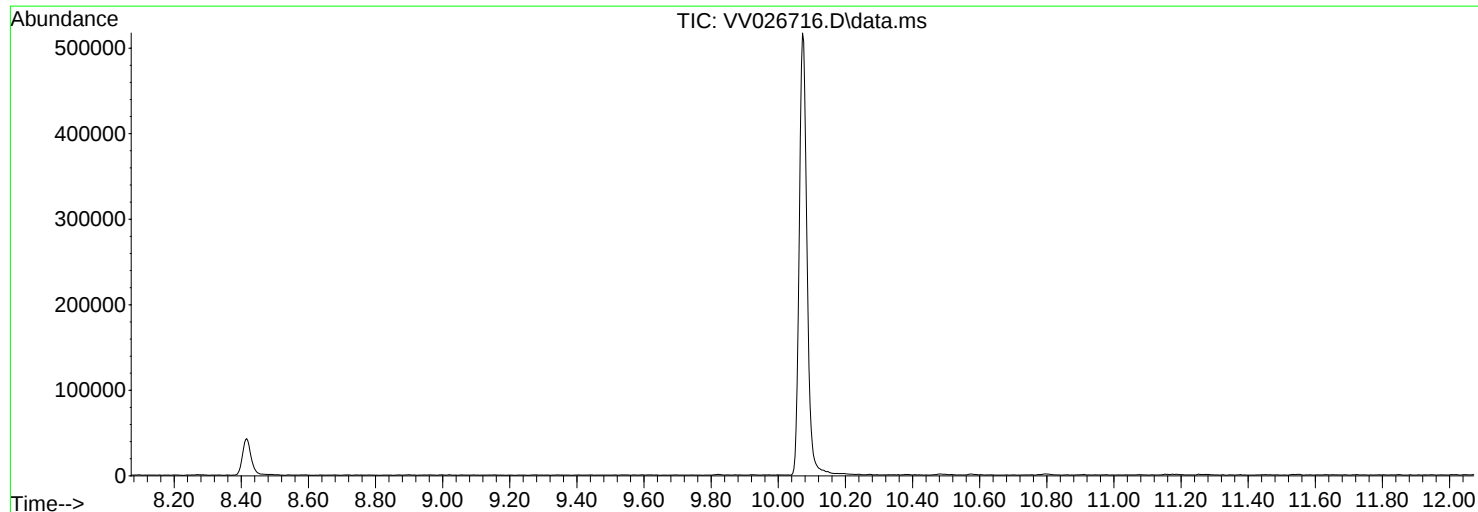

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	17263	PASS
75	95	30	80	49.8	51053	PASS
95	95	100	100	100.0	102608	PASS
96	95	5	9	7.0	7134	PASS
173	174	0.00	2	1.6	1300	PASS
174	95	50	120	78.8	80856	PASS
175	174	5	9	7.5	6101	PASS
176	174	95	105	96.0	77595	PASS
177	176	5	10	6.4	4973	PASS

m/z	Abundance
35.10	110.0
39.90	359.0
44.00	604.0

Instrument :
MSVOA_V
ClientSampleId :
BFB343

m/z	Abundance
35.90	880.0
37.00	4264.0
38.00	3738.0
39.00	1773.0
40.00	508.0
43.00	113.0
44.00	971.0
45.00	911.0
46.20	209.0
47.00	1302.0
47.90	551.0
49.00	3832.0
50.00	16260.0
51.00	5393.0
52.00	277.0
53.10	172.0
53.90	103.0
54.90	304.0
56.00	1607.0
57.00	2559.0
59.90	824.0
61.00	4676.0
62.00	4709.0
63.00	4011.0
63.90	821.0
65.00	1211.0
66.80	222.0
67.20	268.0
68.00	9730.0
69.00	10000.0
70.00	820.0
71.90	563.0
73.00	5101.0
74.10	16187.0
75.00	49792.0
76.10	4244.0
77.00	687.0
77.90	371.0
78.90	4330.0
79.90	1077.0
80.90	4902.0
82.00	1054.0
83.00	117.0
85.80	197.0
87.00	4526.0
88.00	4250.0
90.80	450.0
92.00	2976.0
93.10	4513.0
94.00	11849.0
95.00	99344.0
96.10	7102.0
97.10	219.0
104.00	392.0
104.90	195.0
106.00	569.0
107.00	144.0
107.80	128.0
111.80	172.0
112.80	103.0
115.00	116.0
115.80	306.0
116.90	821.0
118.00	514.0
118.90	908.0
127.90	423.0
128.90	230.0
129.80	420.0
130.90	181.0
137.00	224.0
141.00	883.0
141.90	146.0
143.00	1639.0
144.00	152.0
145.00	833.0
145.90	133.0
147.90	332.0
150.00	152.0
154.80	211.0
156.90	142.0
158.90	126.0
160.90	129.0
170.80	378.0
172.00	1672.0
173.00	1161.0
174.00	74784.0
175.00	5809.0
176.00	72288.0
177.00	4649.0
178.00	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB343

m/z	Abundance
35.90	922.0
37.00	4643.0
38.00	3860.0
39.00	1834.0
40.00	445.0
42.90	118.0
43.90	1017.0
45.00	948.0
46.20	267.0
47.00	1230.0
47.80	682.0
49.00	4067.0
50.00	17704.0
51.00	5464.0
52.00	316.0
53.10	193.0
54.00	111.0
54.90	287.0
56.00	1654.0
57.00	2562.0
57.90	106.0
59.90	911.0
61.00	4989.0
62.00	4920.0
63.00	4270.0
64.00	882.0
65.00	1468.0
66.10	100.0
68.00	10301.0
69.00	10439.0
70.00	947.0
72.00	623.0
73.00	5280.0
74.00	17320.0
75.00	52704.0
76.10	4500.0
77.00	705.0
77.90	443.0
78.90	4519.0
79.90	1235.0
80.90	5179.0
82.00	1210.0
83.10	150.0
85.80	182.0
87.00	4979.0
88.00	5040.0
90.80	458.0
92.00	3289.0
93.10	4843.0
94.00	12800.0
95.00	105960.0
96.10	7417.0
97.00	248.0
104.00	425.0
104.90	236.0
105.90	597.0
107.00	131.0
107.90	107.0
111.90	201.0
112.80	102.0
114.80	125.0
115.90	337.0
116.90	874.0
117.90	569.0
118.90	932.0
127.90	509.0
128.90	215.0
129.80	406.0
131.00	205.0
134.80	122.0
137.00	203.0
141.00	1121.0
141.90	153.0
143.00	1965.0
144.10	143.0
145.00	855.0
147.90	370.0
150.00	185.0
154.80	248.0
157.00	155.0
158.90	139.0
160.90	152.0
170.80	422.0
172.00	1873.0
173.00	1355.0
174.00	83496.0
175.00	6298.0
176.00	80432.0
177.00	5125.0
178.00	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB343

m/z	Abundance
35.90	845.0
37.00	4590.0
38.00	3812.0
39.00	1763.0
40.20	392.0
42.90	131.0
43.90	1040.0
45.00	863.0
46.20	274.0
47.10	1086.0
47.80	674.0
49.00	4051.0
50.00	17824.0
51.00	5242.0
52.00	281.0
53.10	189.0
54.10	113.0
54.90	249.0
56.00	1460.0
57.00	2378.0
57.90	133.0
59.90	925.0
61.00	4693.0
62.00	4798.0
63.00	4255.0
63.90	864.0
65.00	1381.0
66.10	115.0
66.80	176.0
68.00	10003.0
69.00	10364.0
70.10	1028.0
72.00	580.0
73.00	4832.0
74.00	16672.0
75.00	50664.0
76.10	4291.0
77.10	675.0
77.90	480.0
78.90	4404.0
79.90	1196.0
81.00	4874.0
82.00	1175.0
83.10	188.0
85.90	135.0
87.00	4867.0
88.00	5154.0
90.80	461.0
92.00	3324.0
93.00	4685.0
94.00	12232.0
95.00	102520.0
96.00	6883.0
97.00	266.0
104.00	410.0
104.90	227.0
105.80	549.0
111.00	113.0
111.90	167.0
112.80	107.0
114.70	131.0
115.90	335.0
116.90	887.0
117.90	518.0
118.90	914.0
127.90	538.0
128.90	197.0
129.90	376.0
131.00	202.0
134.90	139.0
137.00	167.0
141.00	1252.0
141.80	186.0
143.00	2029.0
144.00	114.0
144.90	839.0
145.70	173.0
147.80	333.0
150.00	165.0
154.80	270.0
157.10	196.0
158.90	137.0
160.90	155.0
170.90	376.0
172.00	1796.0
173.00	1385.0
174.00	84288.0
175.00	6196.0
176.00	80064.0
177.00	5146.0
178.00	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB343