

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071224\
 Data File : VV036501.D
 Acq On : 12 Jul 2024 12:22
 Operator : SY/MD
 Sample : P3215-01
 Misc : 5.86g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4BD3

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 07/16/2024
 Supervised By :Semsettin Yesilyurt 07/16/2024

Quant Time: Jul 13 04:08:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 13 04:06:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	452425	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	396452	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	116777	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	159964	24.679	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.720%
7) Chloroethane-d5	1.529	69	134331	23.704	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.800%
11) 1,1-Dichloroethene-d2	2.053	65	75320	22.629	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	90.520%
21) 2-Butanone-d5	3.867	46	28019m	25.256	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	50.520%
24) Chloroform-d	4.243	84	269228	20.444	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.760%
26) 1,2-Dichloroethane-d4	4.937	65	127640	19.542	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.160%
32) Benzene-d6	4.953	84	511873	25.880	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.520%
36) 1,2-Dichloropropane-d6	5.986	67	146308	24.821	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.280%
41) Toluene-d8	7.239	98	431149	23.626	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.520%
43) trans-1,3-Dichloroprop...	7.551	79	47610	19.427	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.720%
47) 2-Hexanone-d5	8.037	63	14121	21.570	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	43.140%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	87414	17.608	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	70.440%
66) 1,2-Dichlorobenzene-d4	11.558	152	87625	22.111	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.440%
Target Compounds						Qvalue
16) Methylene chloride	2.442	84	25643	2.757	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071224\
Data File : VV036501.D
Acq On : 12 Jul 2024 12:22
Operator : SY/MD
Sample : P3215-01
Misc : 5.86g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 7 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
A4BD3

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/16/2024
Supervised By :Semsettin Yesilyurt 07/16/2024


Quant Time: Jul 13 04:08:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 13 04:06:53 2024
Response via : Initial Calibration

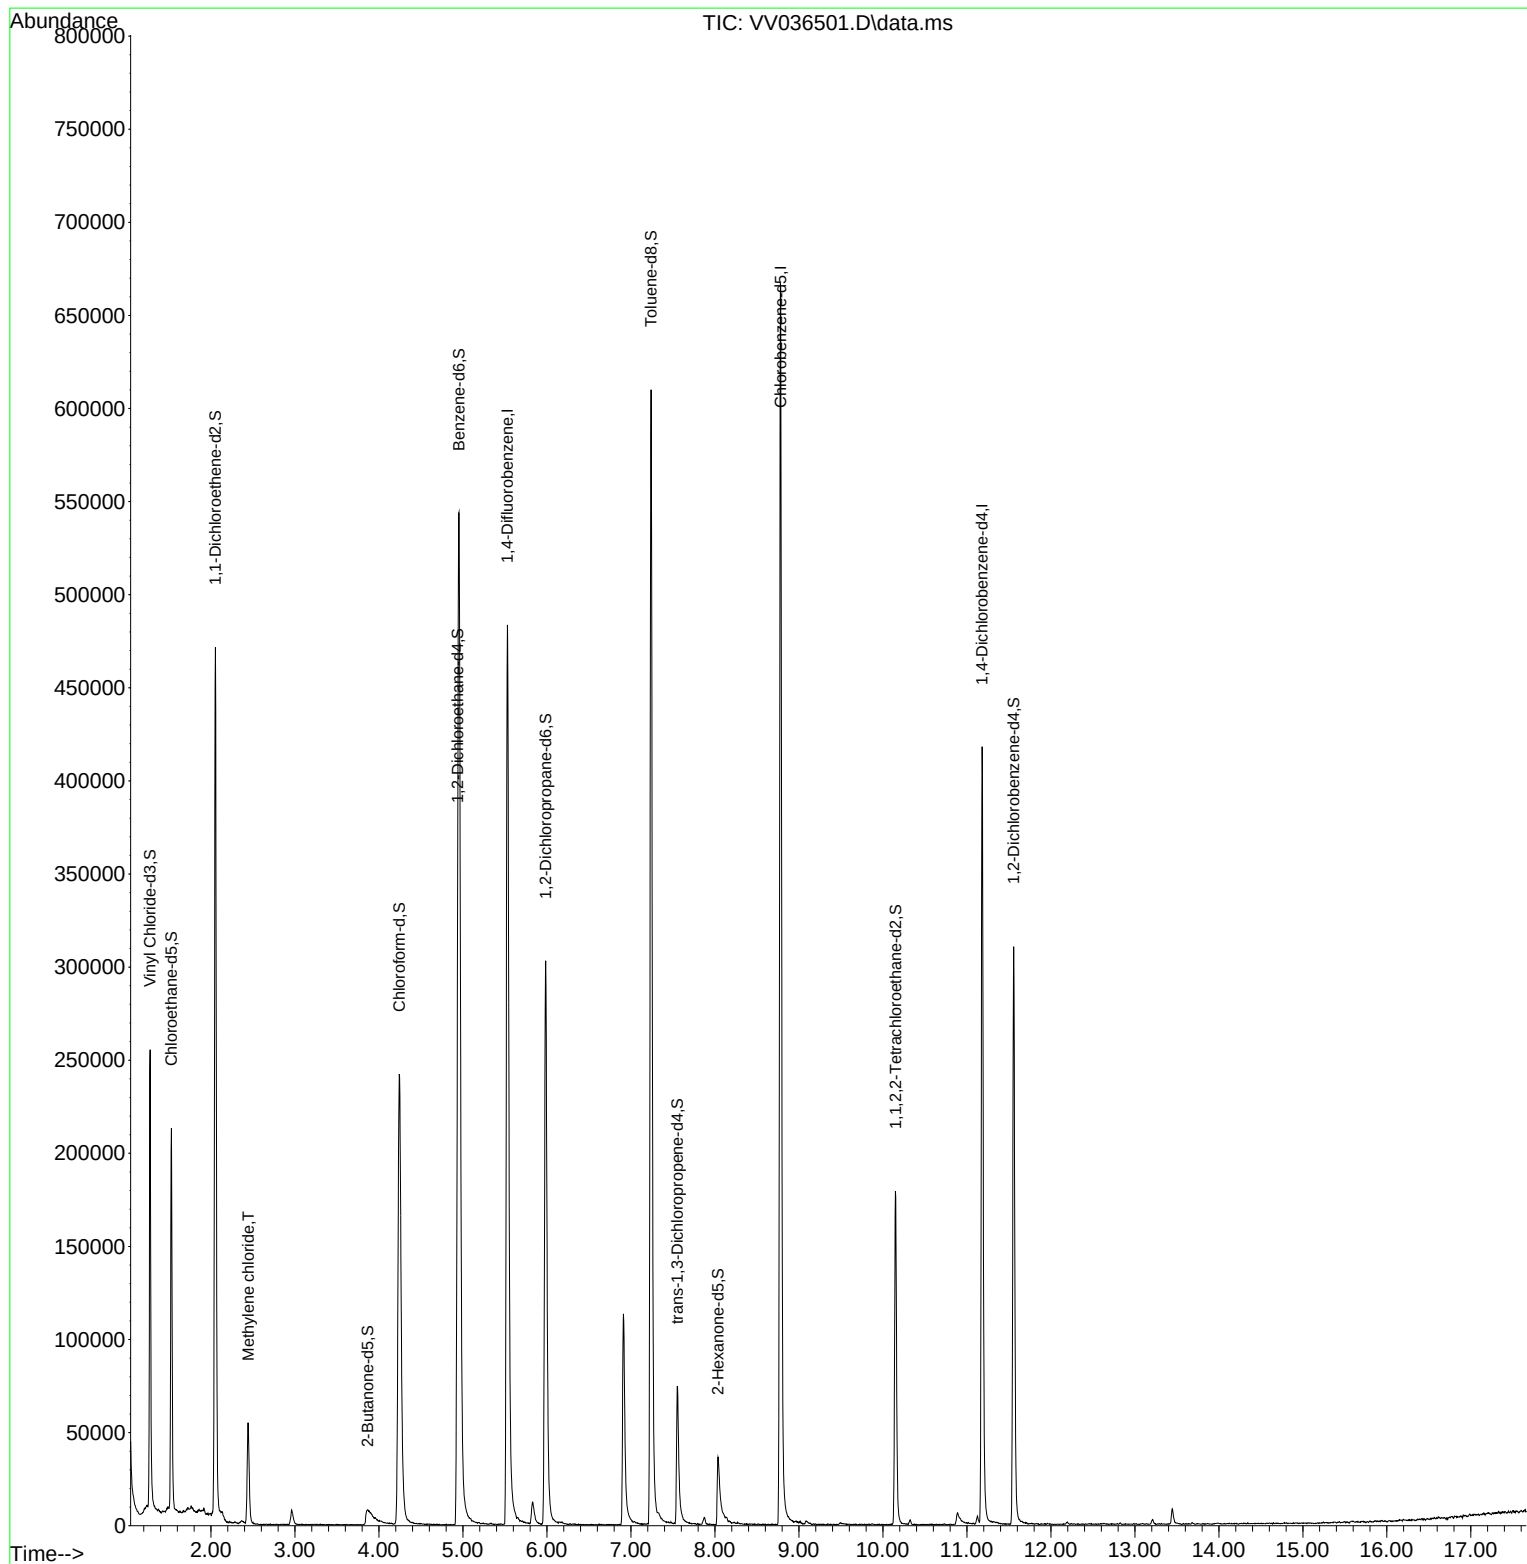

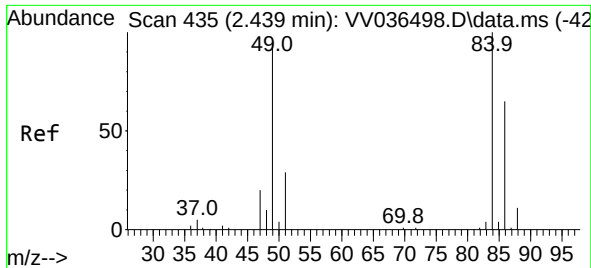

#16
Methylene chloride
Concen: 2.757 ug/L
RT: 2.442 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV036501.D
Acq: 12 Jul 2024 12:22

Instrument :
MSVOA_V
ClientSampleId :
A4BD3

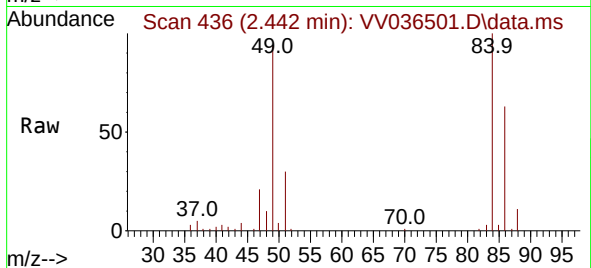

Tgt Ion: 84 Resp: 2564
Ion Ratio Lower Upper
84 100
86 62.6 46.3 86.1
49 94.3 68.1 126.5

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/16/2024
Supervised By :Semsettin Yesilyurt 07/16/2024

