

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
 Data File : VV036522.D
 Acq On : 15 Jul 2024 13:04
 Operator : SY/MD
 Sample : P3215-05
 Misc : 5.64g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 16 01:26:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 16 01:25:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	397520	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	278801	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	60100	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	144693	25.406	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.640%
7) Chloroethane-d5	1.526	69	121621	24.425	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.720%
11) 1,1-Dichloroethene-d2	2.047	65	65727	22.474	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	89.880%
21) 2-Butanone-d5	3.841	46	21117	21.664	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	43.320%
24) Chloroform-d	4.243	84	232555	20.098	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.400%
26) 1,2-Dichloroethane-d4	4.937	65	121056	21.094	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.360%
32) Benzene-d6	4.953	84	421413	30.298	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	121.200%
36) 1,2-Dichloropropane-d6	5.985	67	126495	30.516	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	122.080%#
41) Toluene-d8	7.239	98	308740	24.057	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.240%
43) trans-1,3-Dichloroprop...	7.555	79	37209	21.590	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.360%
47) 2-Hexanone-d5	8.037	63	12244	26.595	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	53.180%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	80378	23.023	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.080%
66) 1,2-Dichlorobenzene-d4	11.561	152	52483	25.732	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.920%
Target Compounds						Qvalue
16) Methylene chloride	2.439	84	26098	3.193	ug/L	94
37) 1,2-Dichloropropane	5.985	63	14345	4.120	ug/L #	84
61) 1,2,3-Trichloropropane	11.181	75	6032	5.641	ug/L #	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
Data File : VV036522.D
Acq On : 15 Jul 2024 13:04
Operator : SY/MD
Sample : P3215-05
Misc : 5.64g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jul 16 01:26:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 01:25:30 2024
Response via : Initial Calibration

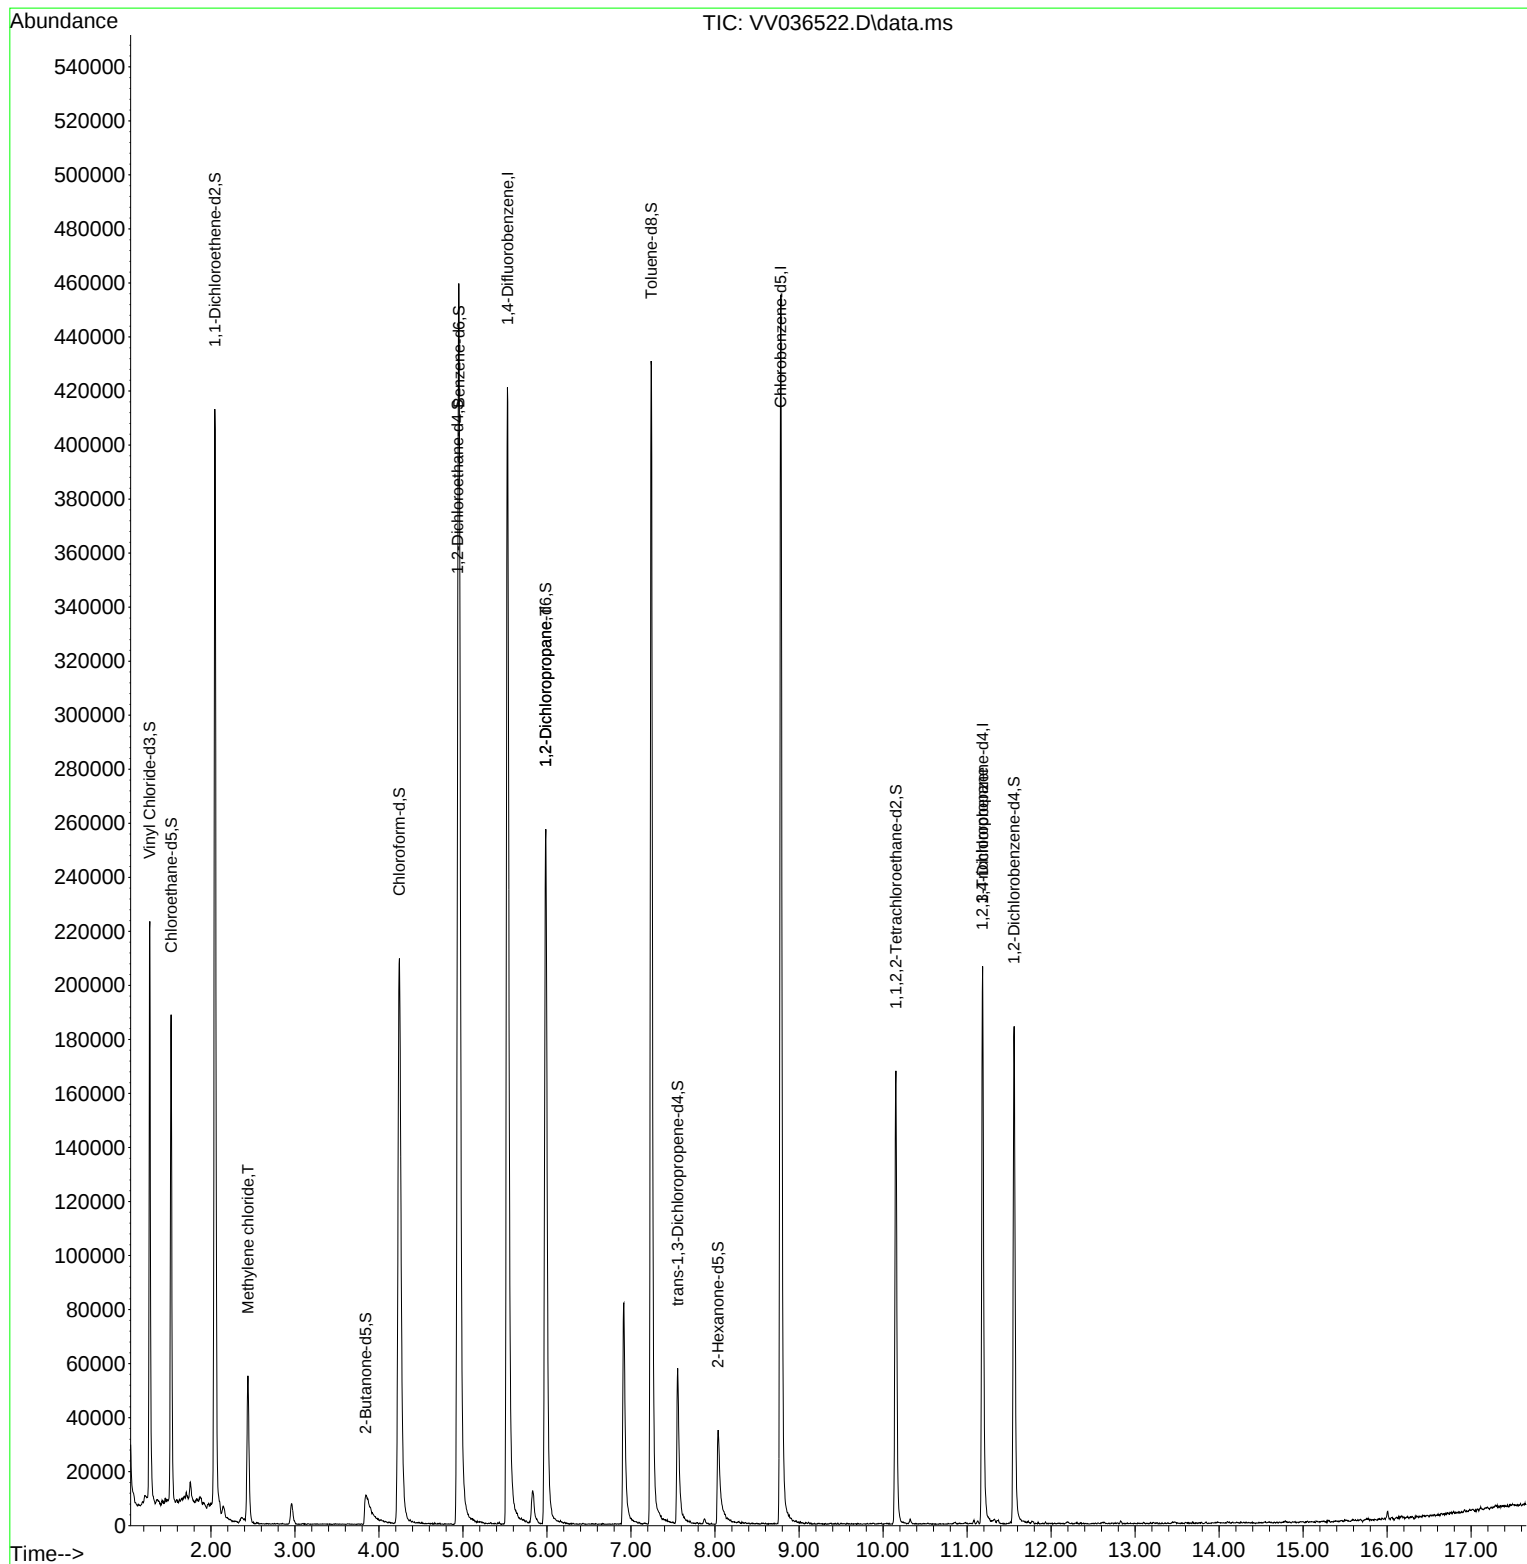



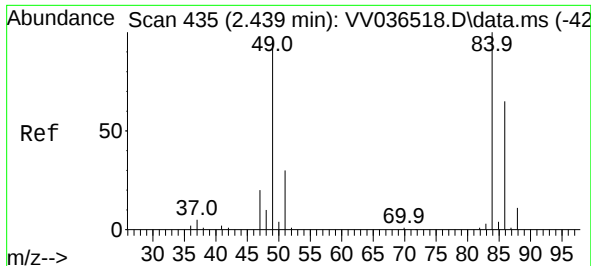


#16
Methylene chloride
Concen: 3.193 ug/L
RT: 2.439 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV036522.D
Acq: 15 Jul 2024 13:04

Instrument :
MSVOA_V
ClientSampleId :



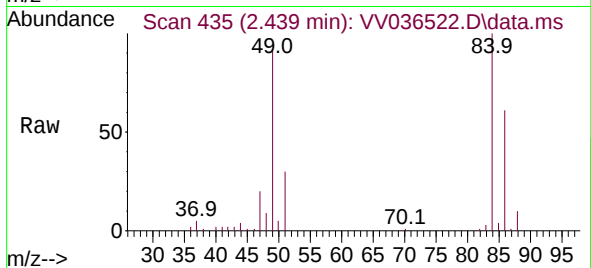



Tgt Ion: 84 Resp: 26098
Ion Ratio Lower Upper
84 100
86 60.8 46.3 86.1
49 91.5 68.1 126.5

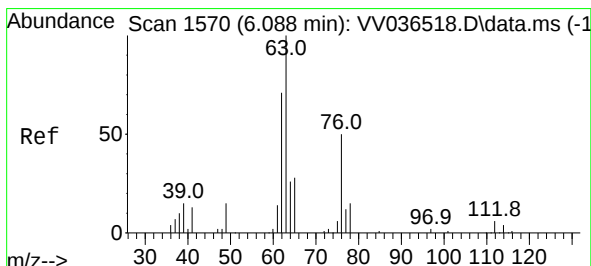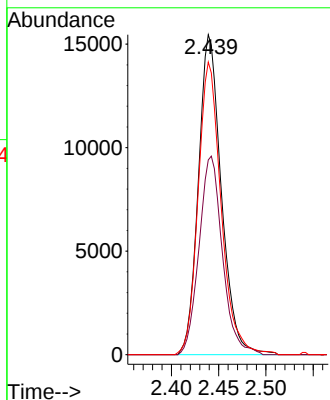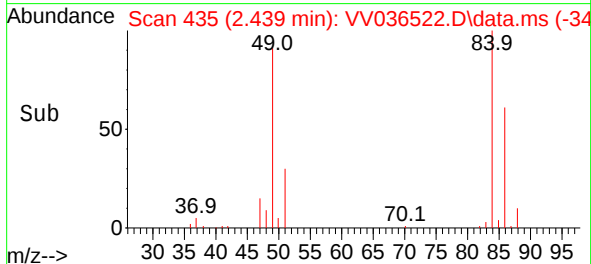

#37
1,2-Dichloropropane
Concen: 4.120 ug/L
RT: 5.985 min Scan# 1538
Delta R.T. -0.103 min
Lab File: VV036522.D
Acq: 15 Jul 2024 13:04


Tgt Ion: 63 Resp: 14345
Ion Ratio Lower Upper
63 100
112 0.3 4.5 6.7#

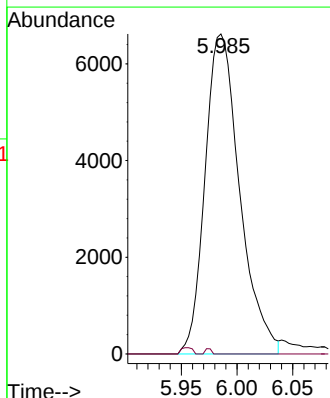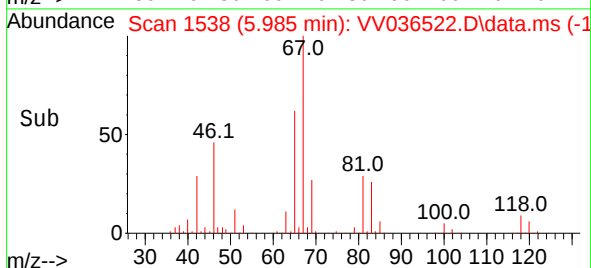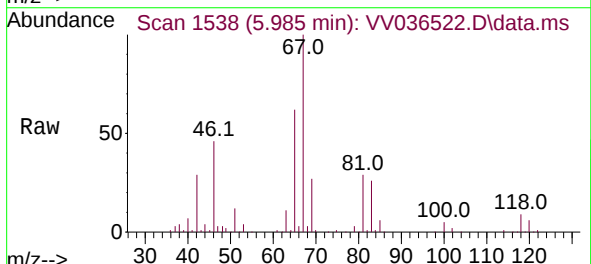

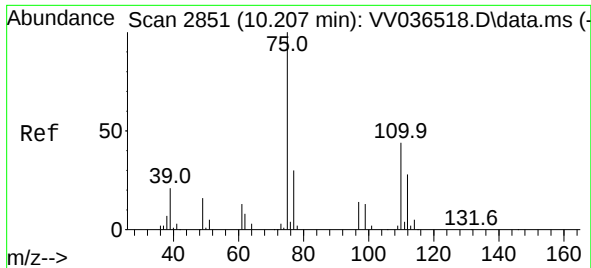

#61
 1,2,3-Trichloropropane
 Concen: 5.641 ug/L
 RT: 11.181 min Scan# 3154
 Delta R.T. 0.974 min
 Lab File: VV036522.D
 Acq: 15 Jul 2024 13:04

Instrument :
 MSVOA_V
 ClientSampleId :

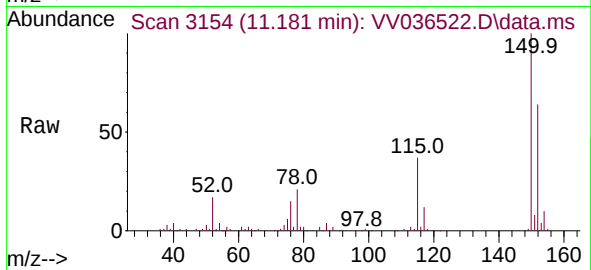

Tgt Ion:	75	Resp:	6032
Ion	Ratio	Lower	Upper
75	100		
77	34.7	25.6	38.4
110	1.1	34.8	52.2#

