




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
Data File : VV036527.D
Acq On : 15 Jul 2024 15:01
Operator : SY/MD
Sample : P3215-13 RE
Misc : 5.02g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4D26RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:28:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 01:25:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/16/2024
Supervised By :Mahesh Dadoda 07/19/2024

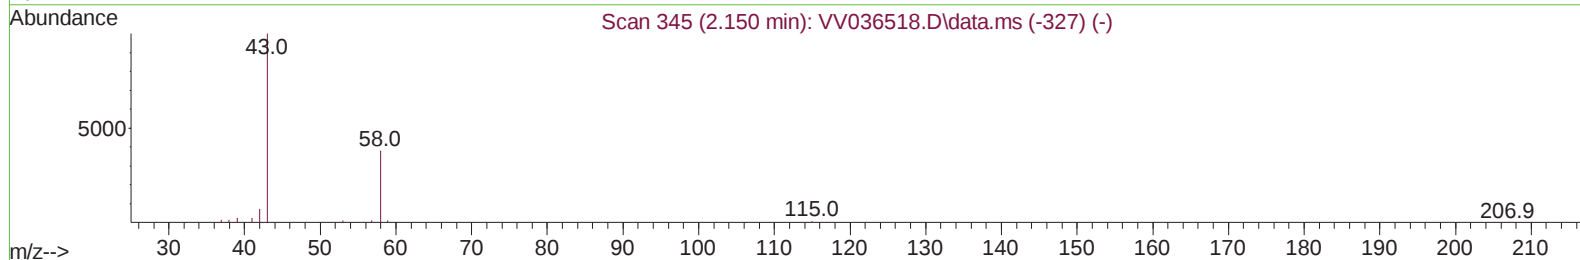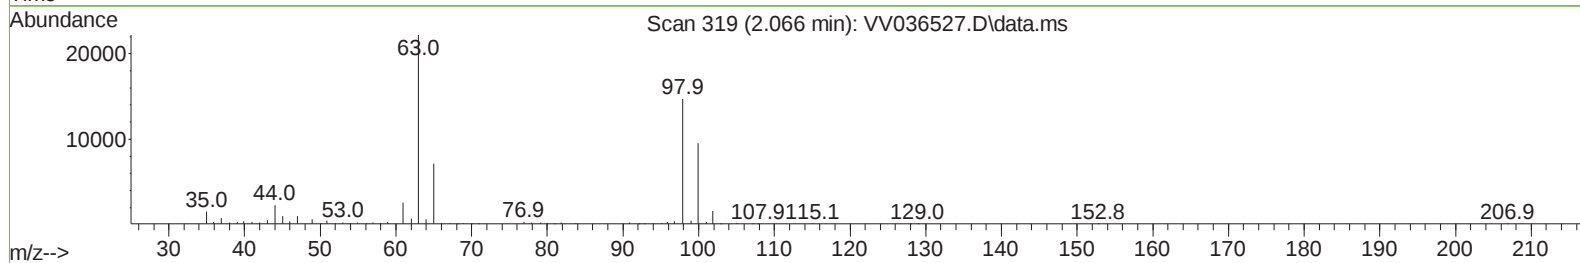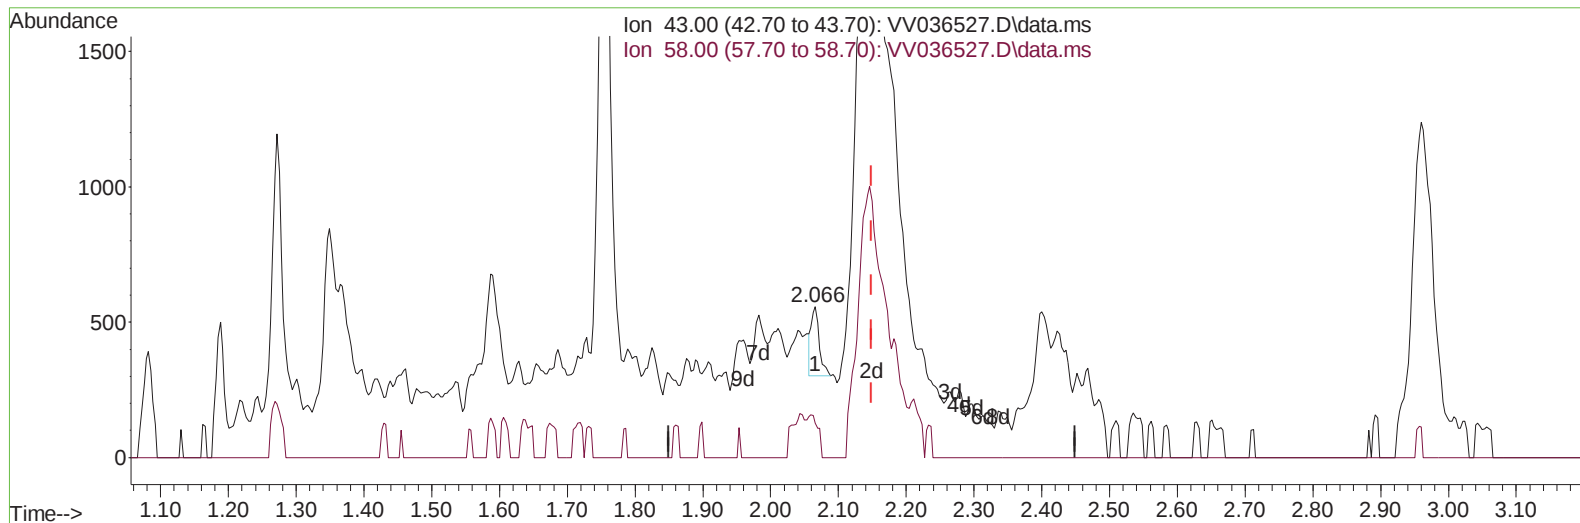

TIC: VV036527.D\data.ms

(13) Acetone (T)

2.066min (-0.084) 0.27 ug/L

response 209

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.20	11.48
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
Data File : VV036527.D
Acq On : 15 Jul 2024 15:01
Operator : SY/MD
Sample : P3215-13 RE
Misc : 5.02g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4D26RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:28:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 01:25:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/16/2024
Supervised By :Mahesh Dadoda 07/19/2024

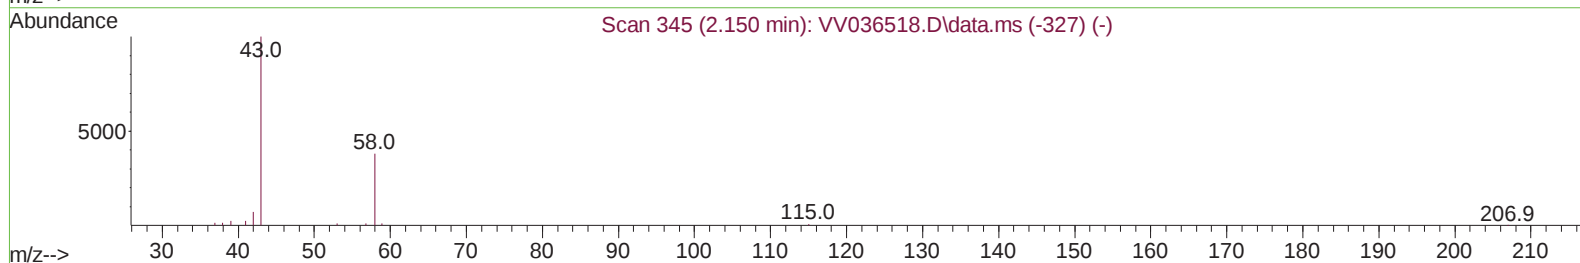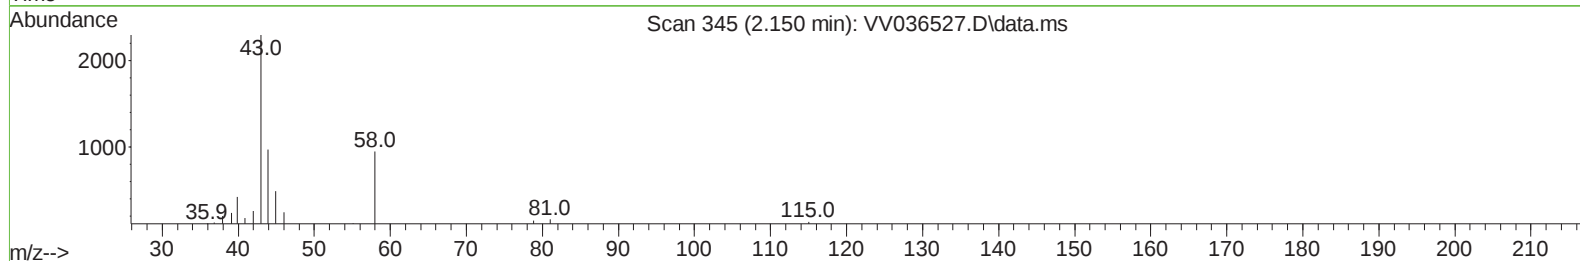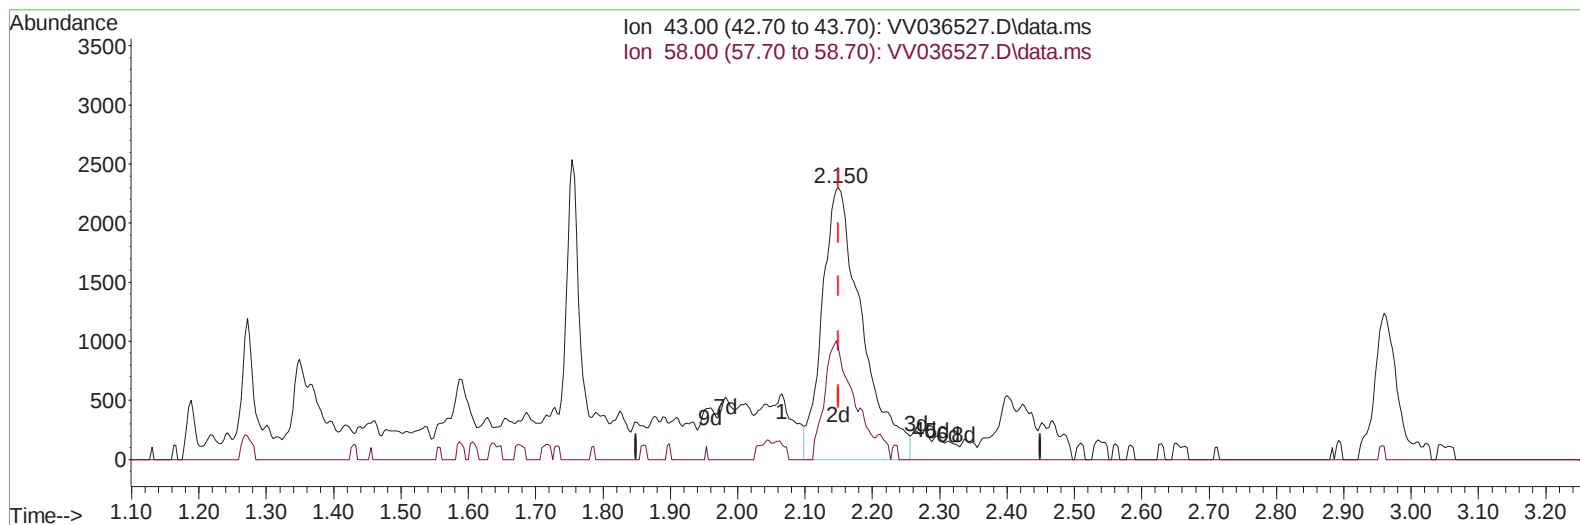

TIC: VV036527.D\data.ms

(13) Acetone (T)

2.150min (-0.000) 12.02 ug/L m

response 9440

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.20	0.25
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
 Data File : VV036527.D
 Acq On : 15 Jul 2024 15:01
 Operator : SY/MD
 Sample : P3215-13 RE
 Misc : 5.02g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4D26RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:28:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 16 01:25:30 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/16/2024
 Supervised By :Mahesh Dadoda 07/19/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.532	114		226453	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		94784	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152		10712	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.272	65		144174	44.438	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	= 177.760%#		
7) Chloroethane-d5	1.526	69		124218	43.792	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	= 175.160%#		
11) 1,1-Dichloroethene-d2	2.047	65		55715	33.442	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	= 133.760%#		
21) 2-Butanone-d5	3.831	46		31019	55.861	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	= 111.720%		
24) Chloroform-d	4.243	84		230939	35.036	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	= 140.160%		
26) 1,2-Dichloroethane-d4	4.937	65		105577	32.293	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	= 129.160%		
32) Benzene-d6	4.953	84		384011	81.210	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	= 324.840%#		
36) 1,2-Dichloropropane-d6	5.985	67		126953	90.085	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	= 360.320%#		
41) Toluene-d8	7.243	98		187893	43.065	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	= 172.240%#		
43) trans-1,3-Dichloroprop...	7.561	79		15705	26.804	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	= 107.200%		
47) 2-Hexanone-d5	8.034	63		14664	93.688	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	= 187.380%#		
56) 1,1,2,2-Tetrachloroeth...	10.152	84		73819	62.196	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	= 248.800%#		
66) 1,2-Dichlorobenzene-d4	11.564	152		14633	40.253	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	= 161.000%#		
Target Compounds							
						Qvalue	
13) Acetone	2.150	43		9440m	12.024	ug/L	
14) Carbon disulfide	2.230	76		7811	1.040	ug/L	99
16) Methylene chloride	2.442	84		33150	7.120	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071524\
Data File : VW036527.D
Acq On : 15 Jul 2024 15:01
Operator : SY/MD
Sample : P3215-13 RE
Misc : 5.02g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4D26RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:28:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 01:25:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/16/2024
Supervised By :Mahesh Dadoda 07/19/2024

