




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
 Data File : VV036539.D
 Acq On : 15 Jul 2024 19:40
 Operator : SY/MD
 Sample : P3238-05
 Misc : 5.84g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4BE8

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:31:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 16 01:25:30 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/16/2024
 Supervised By :Mahesh Dadoda 07/19/2024

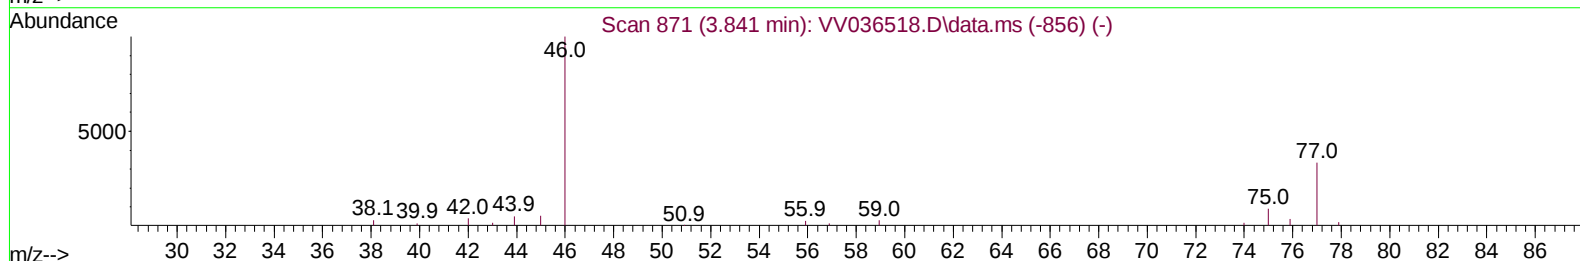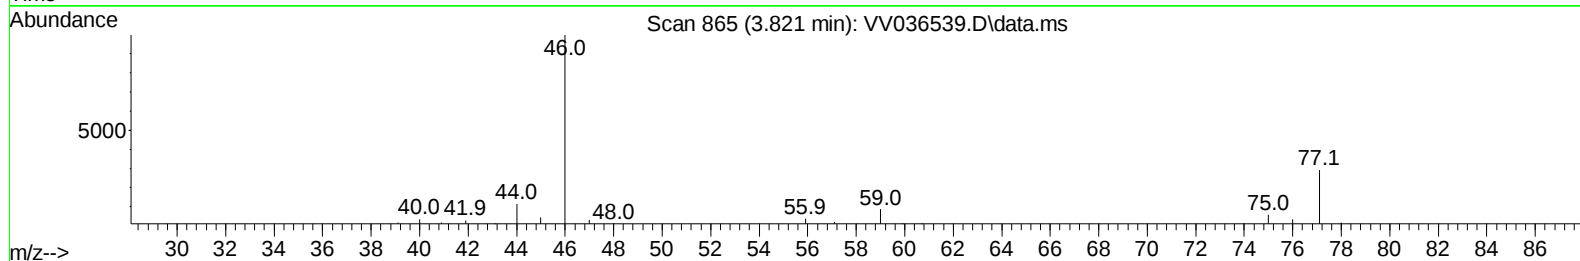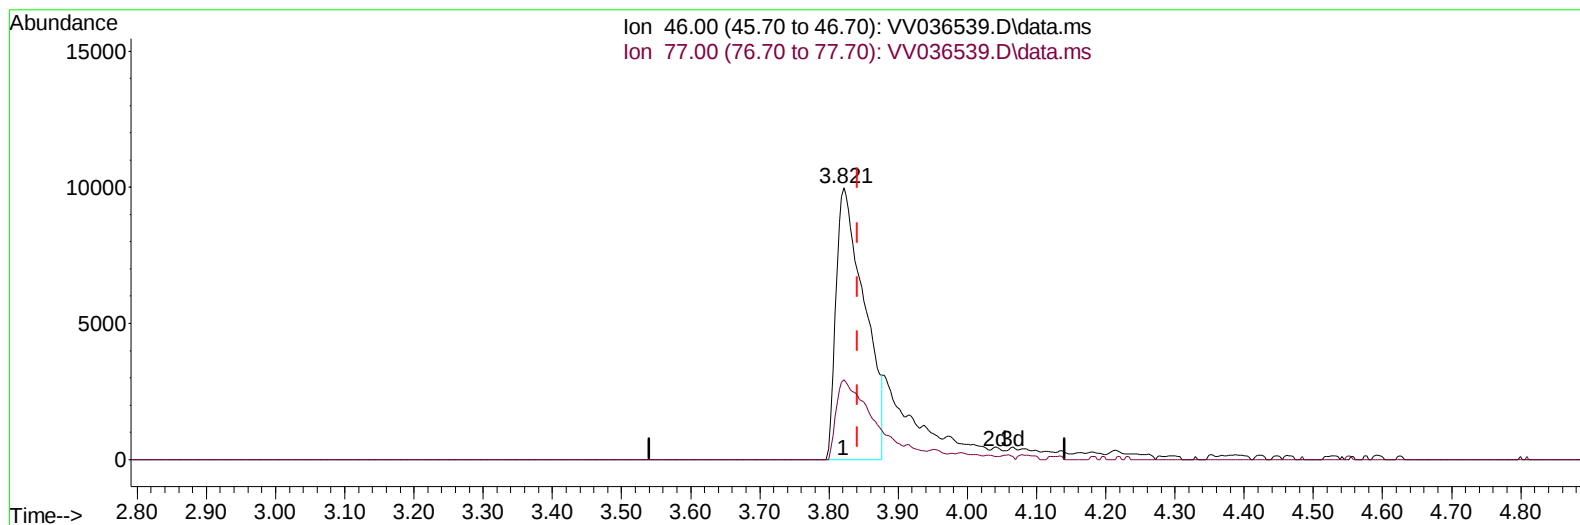

TIC: VV036539.D\data.ms

(21) 2-Butanone-d5 (S)

3.821min (-0.019) 25.78 ug/L

response 28491

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.40	36.54#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
Data File : VV036539.D
Acq On : 15 Jul 2024 19:40
Operator : SY/MD
Sample : P3238-05
Misc : 5.84g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4BE8

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:31:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 01:25:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/16/2024
Supervised By :Mahesh Dadoda 07/19/2024

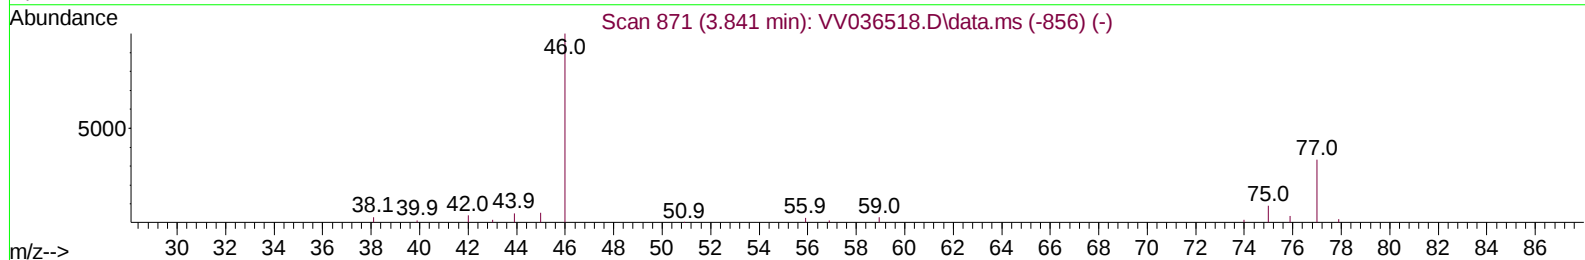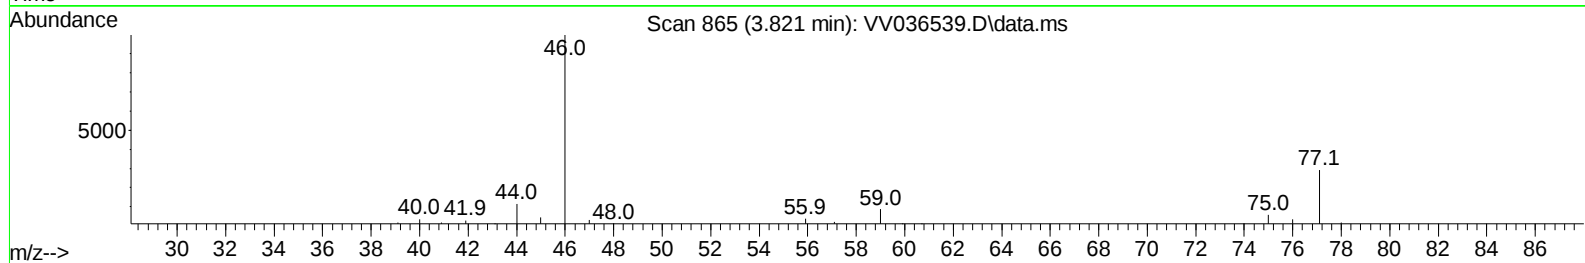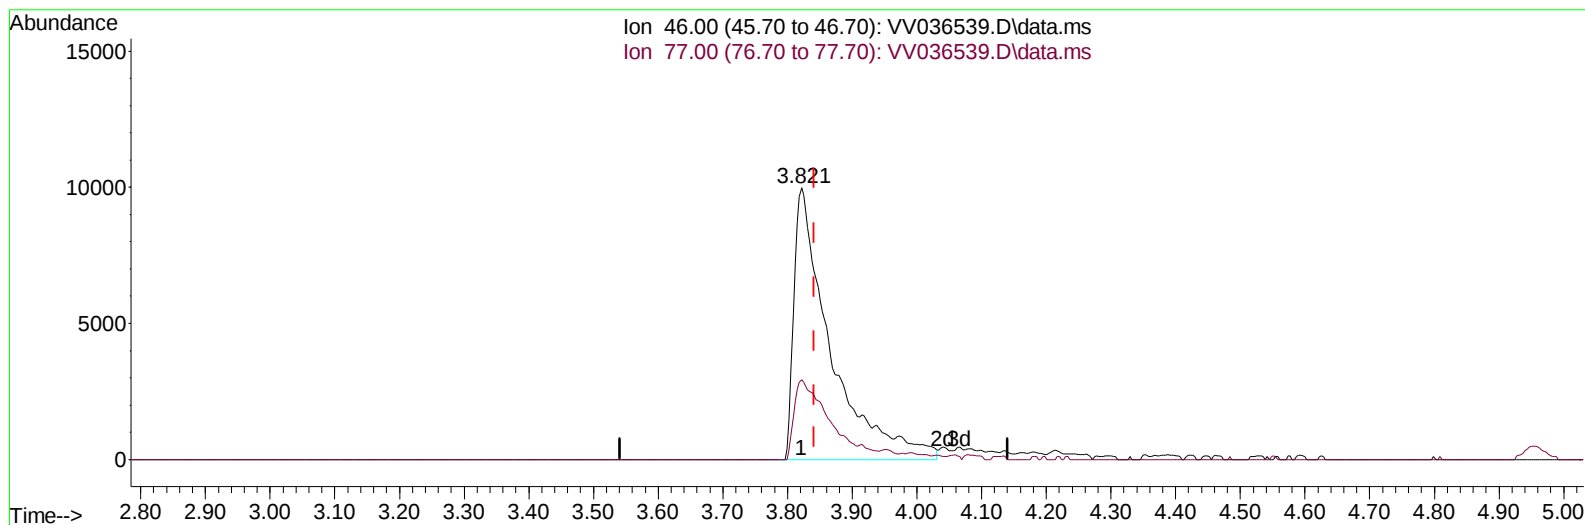

TIC: VV036539.D\data.ms

(21) 2-Butanone-d5 (S)

3.821min (-0.019) 35.37 ug/L m

response 39096

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.40	26.63#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
 Data File : VV036539.D
 Acq On : 15 Jul 2024 19:40
 Operator : SY/MD
 Sample : P3238-05
 Misc : 5.84g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4BE8

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:31:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 16 01:25:30 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/16/2024
 Supervised By :Mahesh Dadoda 07/19/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.529	114		450779	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117		466859	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		203333	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.272	65		142209	22.020	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	88.080%		
7) Chloroethane-d5	1.526	69		127176	22.523	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	90.080%		
11) 1,1-Dichloroethene-d2	2.047	65		64767	19.530	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	78.120%		
21) 2-Butanone-d5	3.821	46		39096m	35.369	ug/L	-0.02
Spiked Amount 50.000	Range 20	- 135		Recovery =	70.740%		
24) Chloroform-d	4.243	84		269323	20.526	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	82.120%		
26) 1,2-Dichloroethane-d4	4.937	65		138099	21.220	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	84.880%		
32) Benzene-d6	4.953	84		505435	21.701	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	86.800%		
36) 1,2-Dichloropropane-d6	5.985	67		147997	21.321	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	85.280%		
41) Toluene-d8	7.239	98		444519	20.685	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	82.720%		
43) trans-1,3-Dichloroprop...	7.551	79		56340	19.522	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	78.080%		
47) 2-Hexanone-d5	8.030	63		27169	35.242	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	70.480%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84		111491	19.071	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	76.280%		
66) 1,2-Dichlorobenzene-d4	11.561	152		170180	24.662	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	98.640%		
Target Compounds							
16) Methylene chloride	2.439	84		64590	6.969	ug/L	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
Data File : VV036539.D
Acq On : 15 Jul 2024 19:40
Operator : SY/MD
Sample : P3238-05
Misc : 5.84g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4BE8

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:31:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 01:25:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/16/2024
Supervised By :Mahesh Dadoda 07/19/2024

