

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
 Data File : VV036523.D
 Acq On : 15 Jul 2024 13:28
 Operator : SY/MD
 Sample : P3215-06RE
 Misc : 4.73g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4C09RE

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 07/16/2024
 Supervised By :Mahesh Dadoda 07/19/2024

Quant Time: Jul 16 01:27:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 16 01:25:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	367692	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	291962	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	70968	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	125552	23.834	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	95.320%		
7) Chloroethane-d5	1.526	69	106568	23.138	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	92.560%		
11) 1,1-Dichloroethene-d2	2.050	65	53687	19.847	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	79.400%		
21) 2-Butanone-d5	3.850	46	18727m	20.770	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	41.540%		
24) Chloroform-d	4.243	84	198851	18.579	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	74.320%		
26) 1,2-Dichloroethane-d4	4.937	65	102015	19.218	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	76.880%		
32) Benzene-d6	4.953	84	330728	22.706	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	90.840%		
36) 1,2-Dichloropropane-d6	5.985	67	105116	24.215	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	96.880%		
41) Toluene-d8	7.243	98	228809	17.025	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	68.120%		
43) trans-1,3-Dichloroprop...	7.558	79	23153	12.829	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	51.320%		
47) 2-Hexanone-d5	8.040	63	6394	13.262	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	26.520%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	60531	16.557	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	66.240%		
66) 1,2-Dichlorobenzene-d4	11.561	152	32991	13.698	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	54.800%#		
Target Compounds						
16) Methylene chloride	2.439	84	34421	4.553	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071524\
Data File : VV036523.D
Acq On : 15 Jul 2024 13:28
Operator : SY/MD
Sample : P3215-06RE
Misc : 4.73g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
A4C09RE

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 07/16/2024
Supervised By :Mahesh Dadoda 07/19/2024


Quant Time: Jul 16 01:27:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 01:25:30 2024
Response via : Initial Calibration

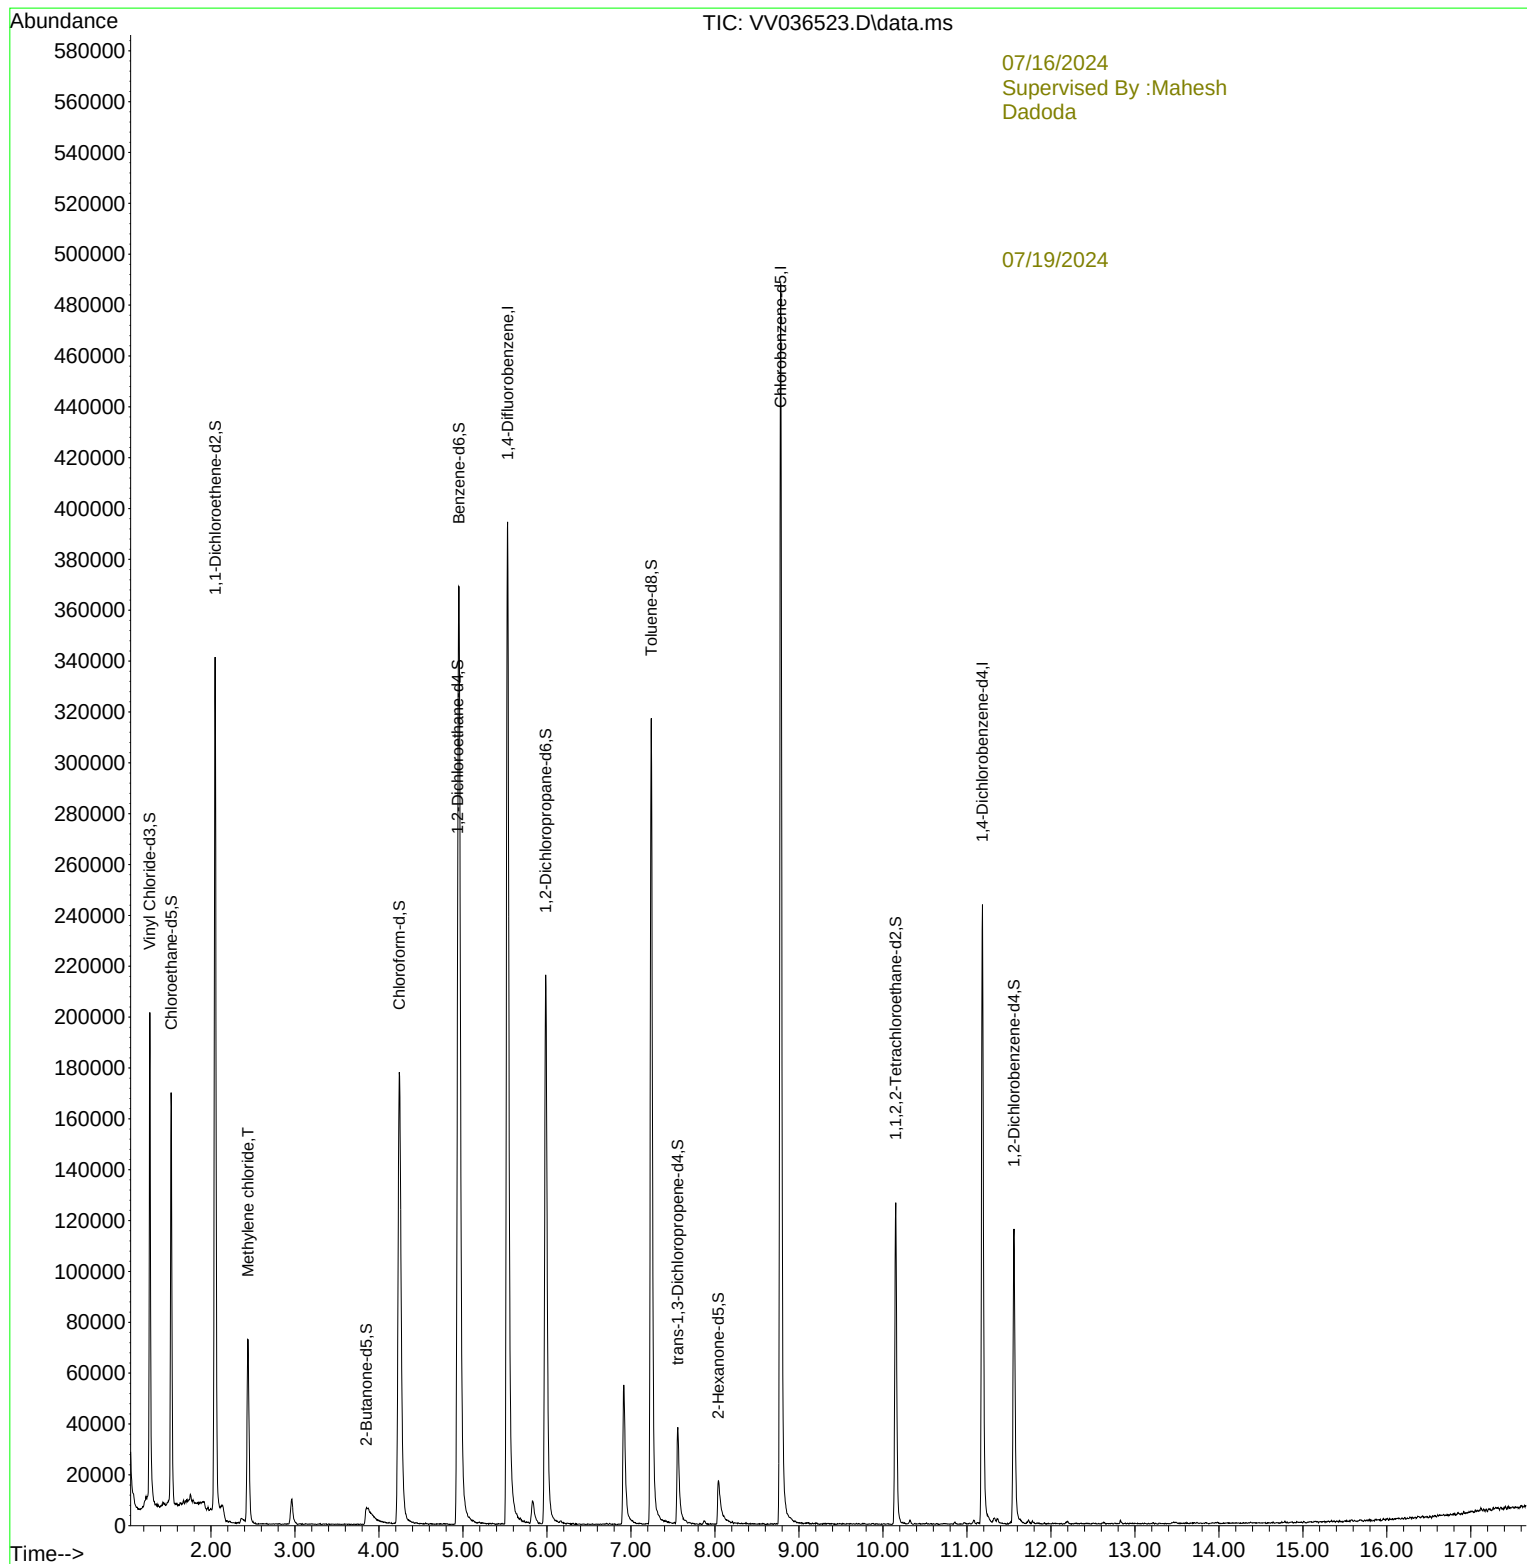

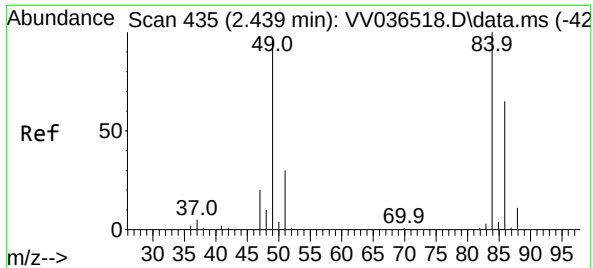

#16
Methylene chloride
Concen: 4.553 ug/L
RT: 2.439 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV036523.D
Acq: 15 Jul 2024 13:28



Instrument : MSVOA_V
ClientSampleId : A4C09RE

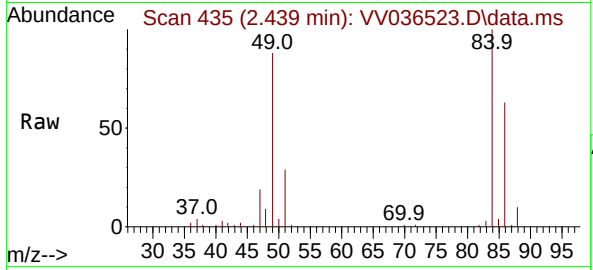

Tgt Ion:	84	Resp:	3442
Ion	Ratio	Lower	Upper
84	100		
86	62.7	46.3	86.1
49	87.9	68.1	126.5

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 07/16/2024
Supervised By :Mahesh Dadoda 07/19/2024

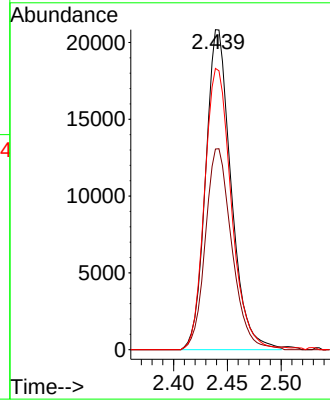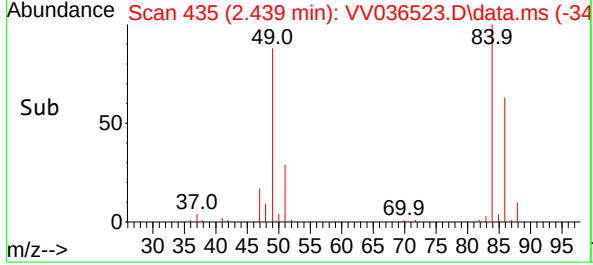

07/16/2024
Supervised By :Mahesh Dadoda

07/19/2024