




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071724\
Data File : VV036591.D
Acq On : 17 Jul 2024 14:20
Operator : SY/MD
Sample : P3238-12
Misc : 5.49g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4BF8

Manual IntegrationsAPPROVED

Quant Time: Jul 18 01:28:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 18 01:25:10 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
Supervised By :Mahesh Dadoda 07/19/2024

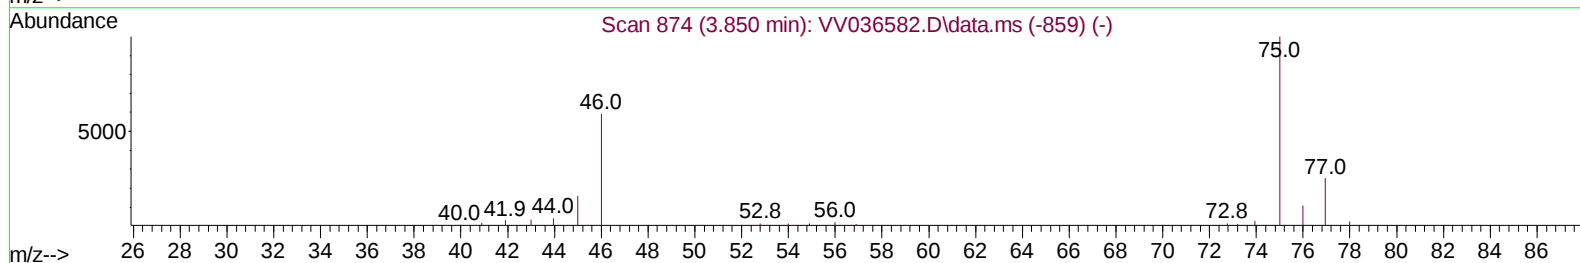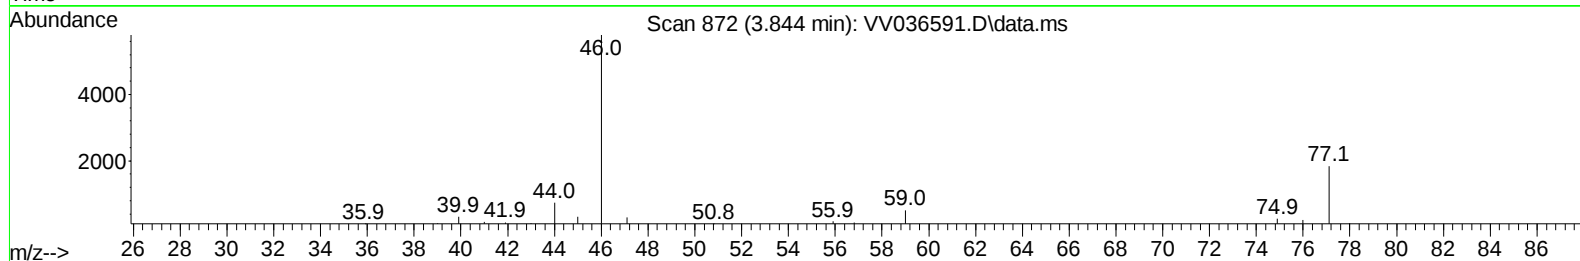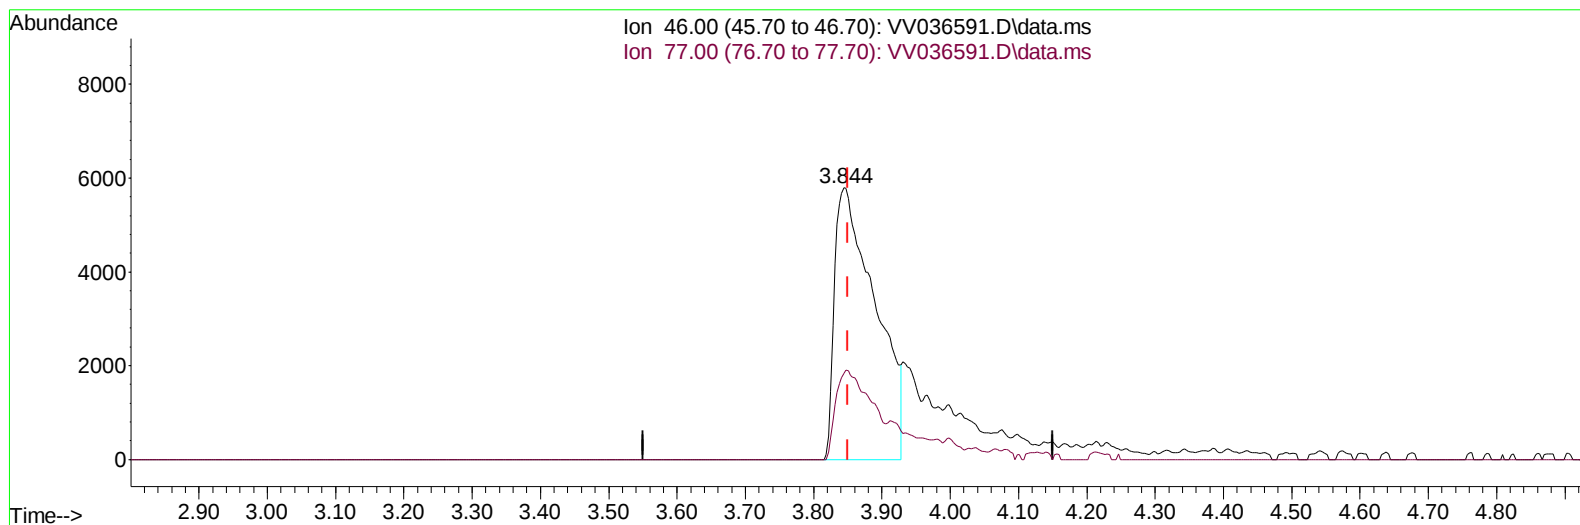

TIC: VV036591.D\data.ms

(21) 2-Butanone-d5 (S)

3.844min (-0.006) 18.50 ug/L

response 24030

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.40	28.44#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071724\
Data File : VV036591.D
Acq On : 17 Jul 2024 14:20
Operator : SY/MD
Sample : P3238-12
Misc : 5.49g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4BF8

Manual IntegrationsAPPROVED

Quant Time: Jul 18 01:28:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 18 01:25:10 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
Supervised By :Mahesh Dadoda 07/19/2024

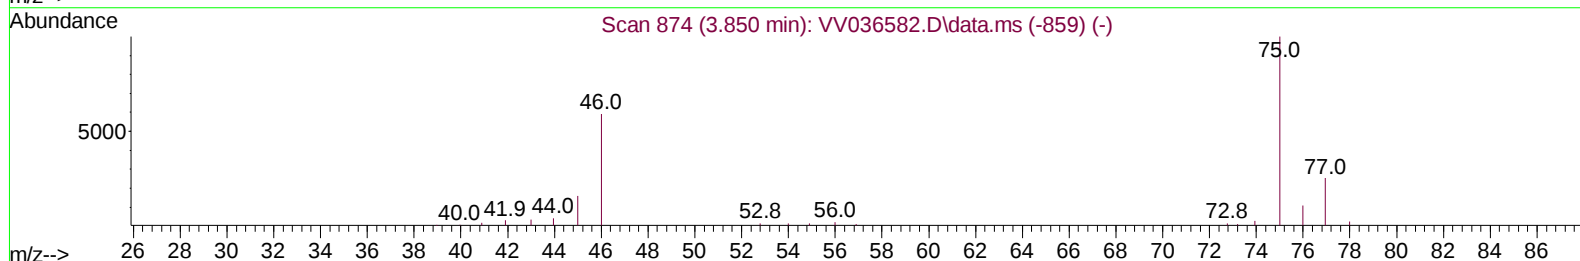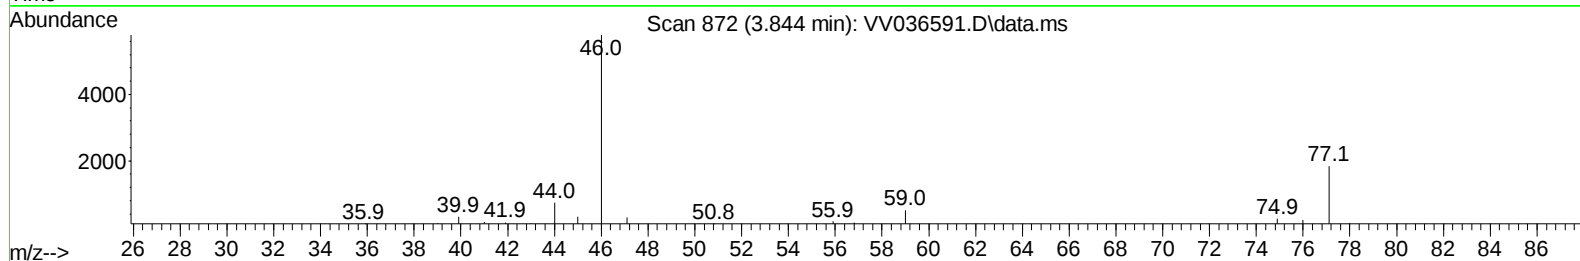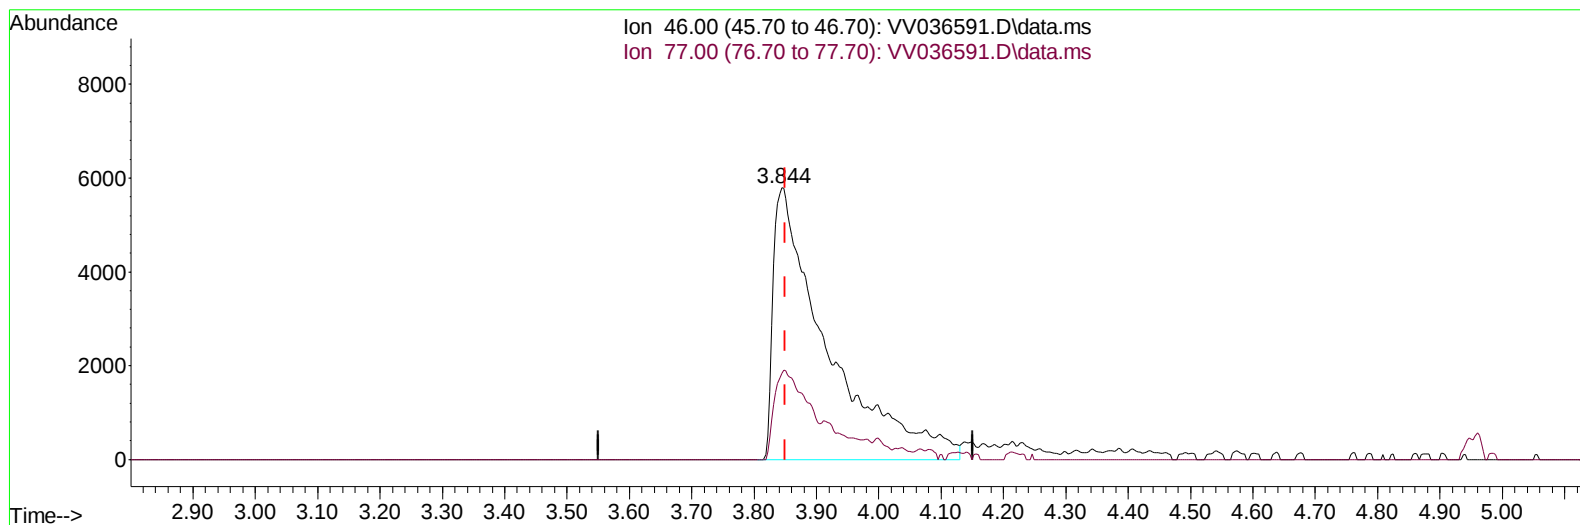

TIC: VV036591.D\data.ms

(21) 2-Butanone-d5 (S)

3.844min (-0.006) 26.85 ug/L m

response 34871

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.40	19.60#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071724\
 Data File : VV036591.D
 Acq On : 17 Jul 2024 14:20
 Operator : SY/MD
 Sample : P3238-12
 Misc : 5.49g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4BF8

Manual IntegrationsAPPROVED

Quant Time: Jul 18 01:28:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 18 01:25:10 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
 Supervised By :Mahesh Dadoda 07/19/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.529	114		529642	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117		515436	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152		182495	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.275	65		141997	18.713	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	74.840%		
7) Chloroethane-d5	1.529	69		120724	18.197	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	72.800%		
11) 1,1-Dichloroethene-d2	2.050	65		69003	17.709	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	70.840%		
21) 2-Butanone-d5	3.844	46		34871m	26.850	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	53.700%		
24) Chloroform-d	4.243	84		260049	16.868	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	67.480%		
26) 1,2-Dichloroethane-d4	4.937	65		126160	16.499	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	66.000%#		
32) Benzene-d6	4.953	84		487746	18.968	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	75.880%		
36) 1,2-Dichloropropane-d6	5.985	67		139442	18.195	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	72.800%		
41) Toluene-d8	7.239	98		427837	18.032	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	72.120%		
43) trans-1,3-Dichloroprop...	7.551	79		49587	15.563	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	62.240%		
47) 2-Hexanone-d5	8.030	63		20437	24.011	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	48.020%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84		96880	15.010	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	60.040%		
66) 1,2-Dichlorobenzene-d4	11.558	152		125126	20.204	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	80.800%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071724\
Data File : VV036591.D
Acq On : 17 Jul 2024 14:20
Operator : SY/MD
Sample : P3238-12
Misc : 5.49g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4BF8

Manual IntegrationsAPPROVED

Quant Time: Jul 18 01:28:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071124SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 18 01:25:10 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
Supervised By :Mahesh Dadoda 07/19/2024

