




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072324\
Data File : VV036648.D
Acq On : 23 Jul 2024 15:53
Operator : SY/MD
Sample : P3276-06
Misc : 9.14g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20H5

Manual IntegrationsAPPROVED

Quant Time: Jul 24 01:01:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 24 00:57:38 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/24/2024
Supervised By :Mahesh Dadoda 07/25/2024

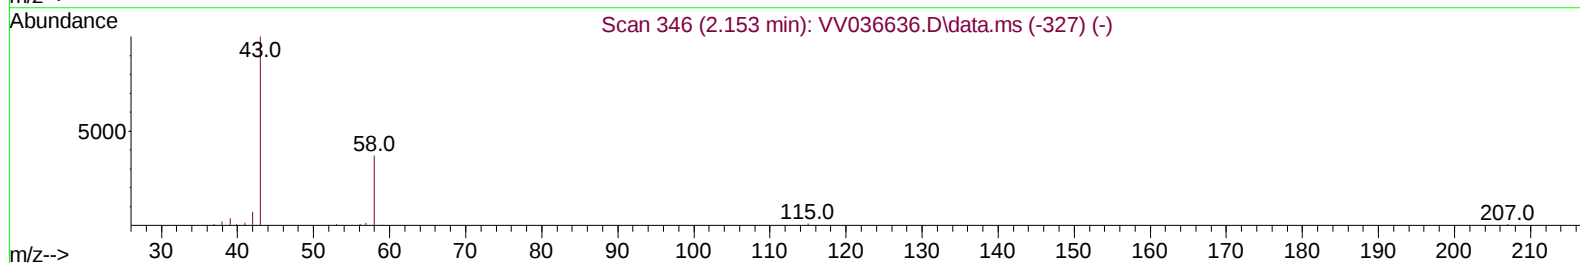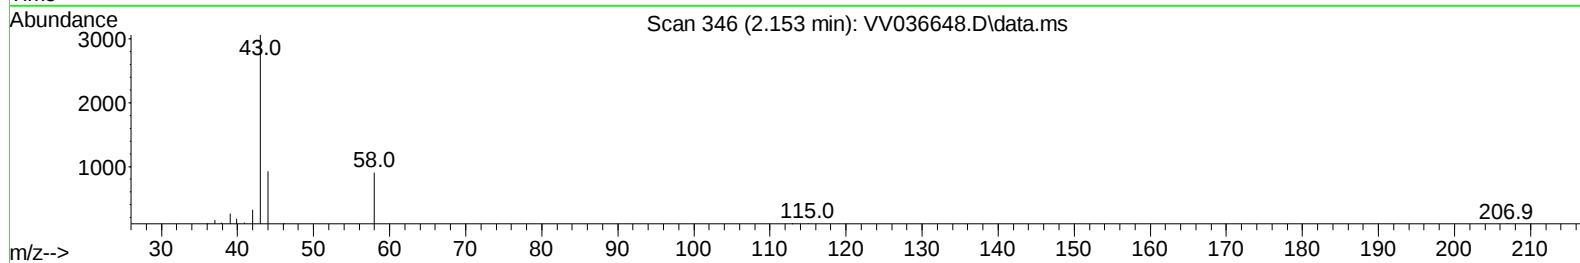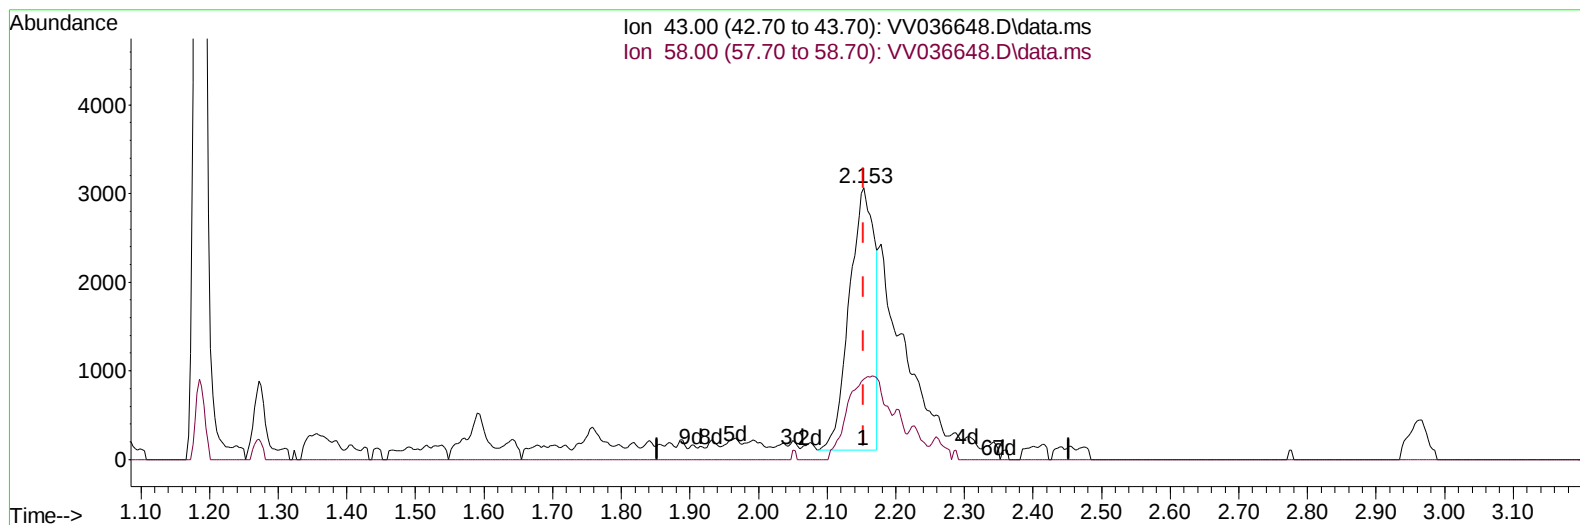

TIC: VV036648.D\data.ms

(13) Acetone (T)

2.153min (+ 0.000) 3.95 ug/L

response 7472

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	11.50	28.95#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072324\
Data File : VV036648.D
Acq On : 23 Jul 2024 15:53
Operator : SY/MD
Sample : P3276-06
Misc : 9.14g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20H5

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 07/24/2024
Supervised By :Mahesh Dadoda 07/25/2024

Quant Time: Jul 24 01:01:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 24 00:57:38 2024
Response via : Initial Calibration

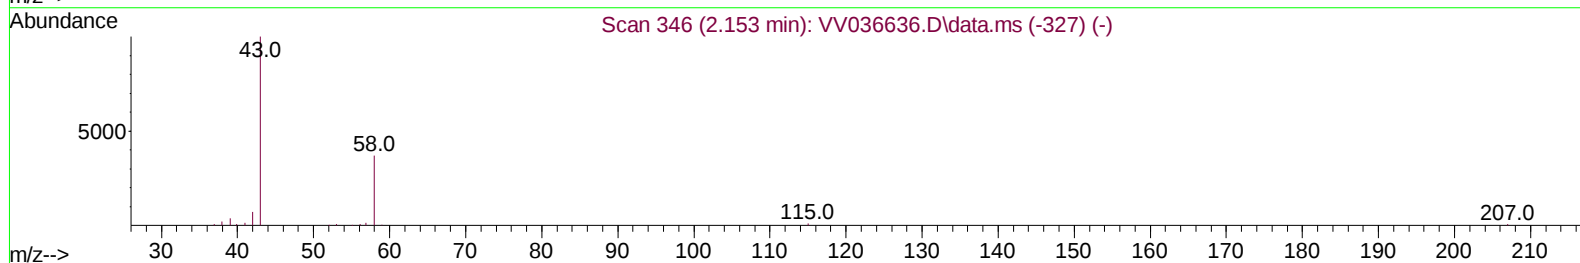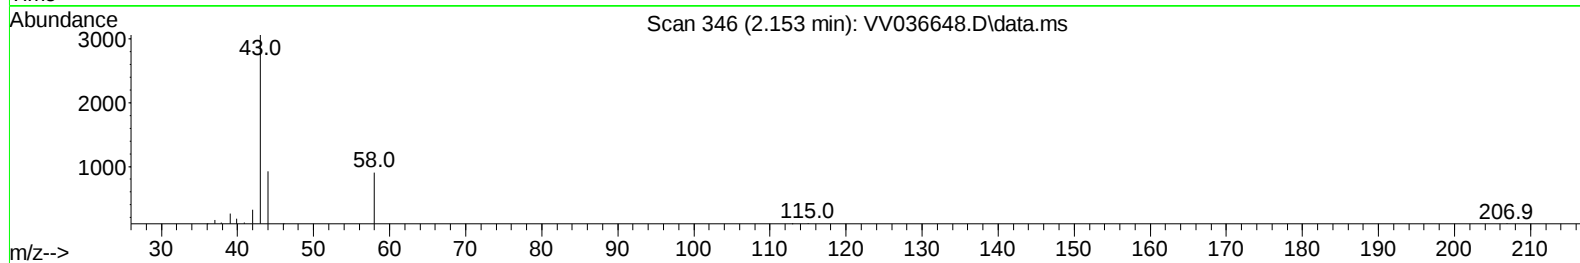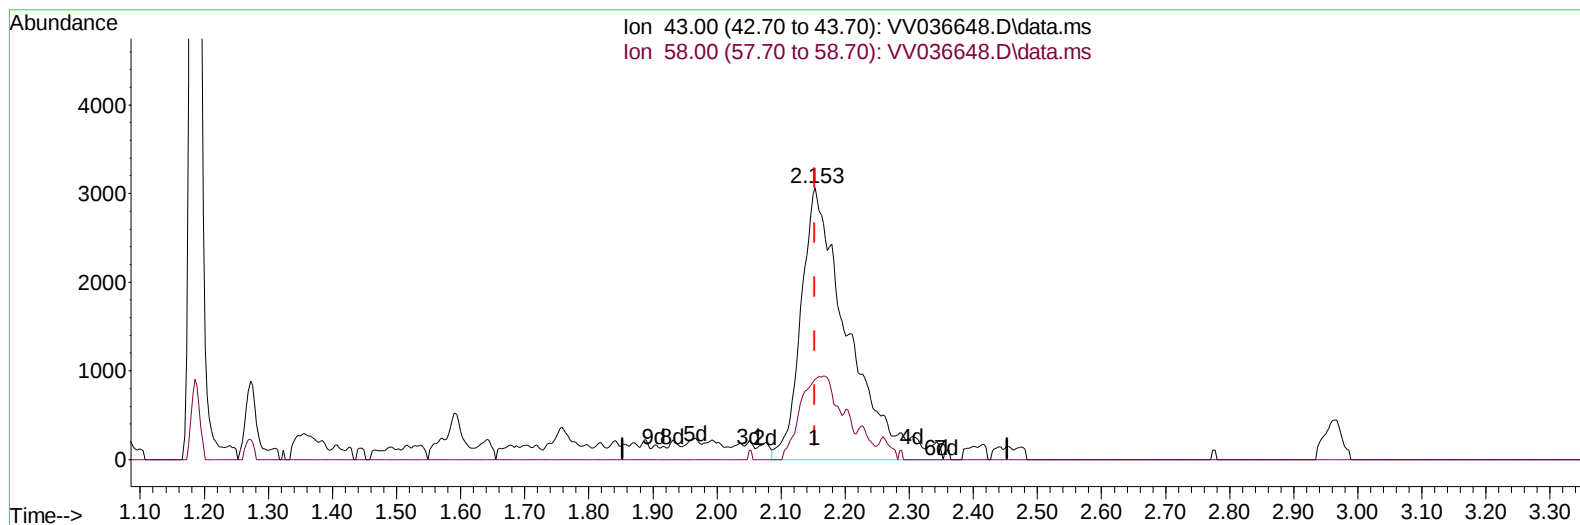

TIC: VV036648.D\data.ms

(13) Acetone (T)

2.153min (+ 0.000) 8.25 ug/L m

response 15606

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	11.50	13.86
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072324\
 Data File : VV036648.D
 Acq On : 23 Jul 2024 15:53
 Operator : SY/MD
 Sample : P3276-06
 Misc : 9.14g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20H5

Manual IntegrationsAPPROVED

Quant Time: Jul 24 01:01:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 24 00:57:38 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/24/2024
 Supervised By :Mahesh Dadoda 07/25/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	455340	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	452248	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	207555	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	51210	10.269	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	41.080%	
7) Chloroethane-d5	1.526	69	55832	12.395	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	49.600%	
11) 1,1-Dichloroethene-d2	2.050	65	26185	9.930	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	39.720%#	
21) 2-Butanone-d5	3.835	46	59405	51.041	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	102.080%	
24) Chloroform-d	4.243	84	190038	15.781	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	63.120%	
26) 1,2-Dichloroethane-d4	4.941	65	113289	19.069	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	76.280%	
32) Benzene-d6	4.953	84	275623	12.859	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	51.440%	
36) 1,2-Dichloropropane-d6	5.986	67	102138	16.724	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	66.880%#	
41) Toluene-d8	7.243	98	224805	10.990	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	43.960%	
43) trans-1,3-Dichloroprop...	7.555	79	45382	16.715	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	66.880%	
47) 2-Hexanone-d5	8.031	63	47929	58.970	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	117.940%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	131629	24.728	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	98.920%	
66) 1,2-Dichlorobenzene-d4	11.558	152	155098	21.406	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	85.640%	
Target Compounds						
13) Acetone	2.153	43	15606m	8.254	ug/L	
34) Trichloroethene	5.844	95	4419	0.526	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072324\
Data File : VV036648.D
Acq On : 23 Jul 2024 15:53
Operator : SY/MD
Sample : P3276-06
Misc : 9.14g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20H5

Manual IntegrationsAPPROVED

Quant Time: Jul 24 01:01:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 24 00:57:38 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/24/2024
Supervised By :Mahesh Dadoda 07/25/2024

