
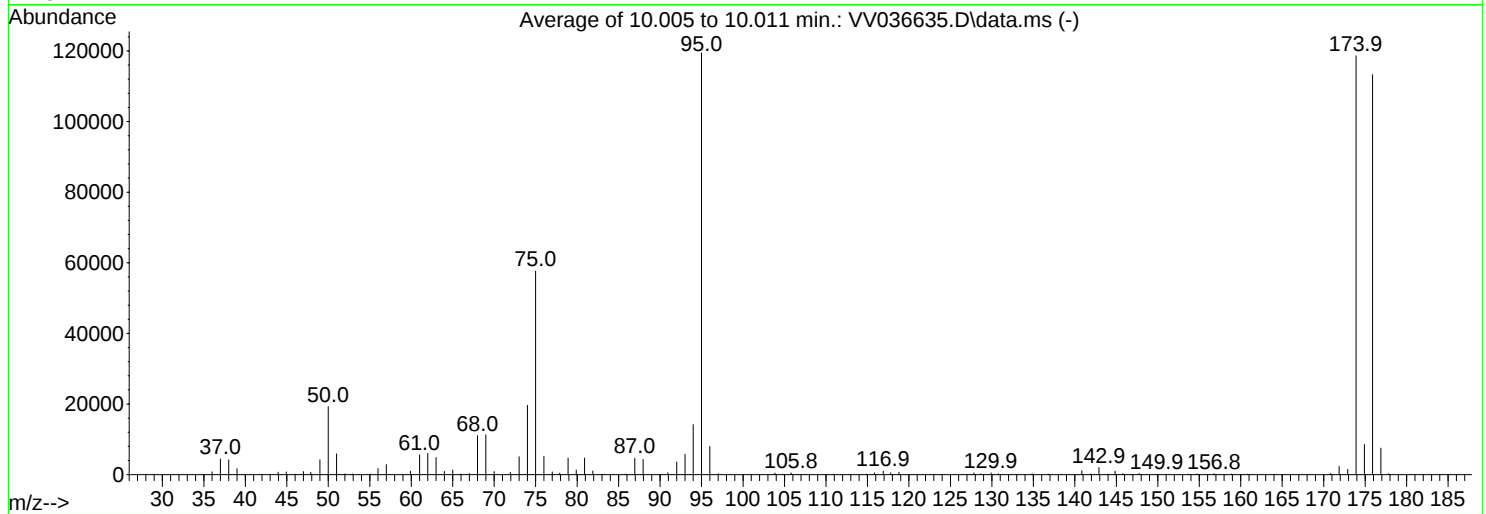


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072324\
Data File : VV036635.D
Acq On : 23 Jul 2024 09:27
Operator : SY/MD
Sample : BFB347
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB347

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Title : VOC Analysis
Last Update : Thu Jul 25 00:49:57 2024

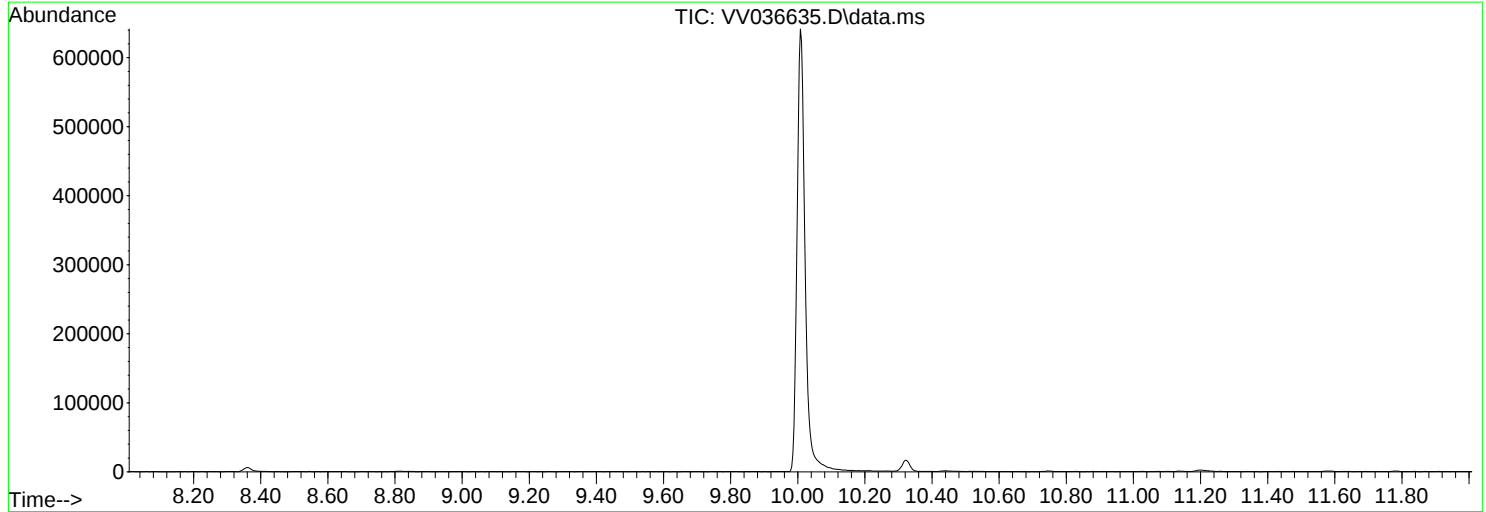

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	19259	PASS
75	95	30	80	48.3	57659	PASS
95	95	100	100	100.0	119459	PASS
96	95	5	9	6.7	7979	PASS
173	174	0.00	2	1.3	1518	PASS
174	95	50	120	99.3	118656	PASS
175	174	5	9	7.2	8527	PASS
176	174	95	101	95.5	113283	PASS
177	176	5	9	6.6	7531	PASS

m/z	Abundance
39.90	176.0
43.90	230.0

Instrument :
MSVOA_V
ClientSampleId :
BFB347

m/z	Abundance
36.00	829.0
37.00	4529.0
38.00	4094.0
39.00	1692.0
39.90	321.0
44.00	967.0
44.90	766.0
46.00	125.0
47.00	814.0
47.90	685.0
49.00	4202.0
50.00	19144.0
51.00	5780.0
52.00	249.0
52.90	195.0
53.80	102.0
54.90	267.0
56.00	1690.0
57.00	2828.0
58.00	155.0
59.90	952.0
61.00	5372.0
62.00	5795.0
63.00	4643.0
64.00	908.0
65.00	1148.0
66.00	171.0
67.00	327.0
68.00	10919.0
69.00	11007.0
70.00	906.0
71.90	605.0
73.00	4939.0
74.00	18952.0
75.00	55752.0
76.00	4998.0
77.00	780.0
77.90	429.0
78.90	4628.0
79.90	1412.0
80.90	4678.0
81.90	1095.0
85.80	111.0
86.10	116.0
87.00	4520.0
87.90	4159.0
90.90	469.0
92.00	3473.0
93.00	5708.0
94.00	13773.0
95.00	115088.0
96.00	7856.0
97.10	258.0
104.00	426.0
104.80	158.0
105.80	464.0
106.70	104.0
108.10	104.0
110.90	136.0
114.90	167.0
115.90	451.0
116.90	942.0
117.80	471.0
118.80	728.0
127.80	486.0
128.70	199.0
129.90	502.0
130.80	196.0
134.80	209.0
136.80	176.0
140.80	1108.0
142.00	193.0
142.90	2038.0
144.00	158.0
144.90	961.0
145.80	322.0
146.80	106.0
147.70	313.0
149.90	136.0
153.70	114.0
154.70	234.0
156.80	256.0
158.90	161.0
160.80	118.0
170.80	310.0
171.80	2162.0
172.90	1431.0
173.90	111848.0
174.90	8296.0
175.90	106384.0
176.90	7229.0
177.90	289.0

Instrument :
MSVOA_V
ClientSampleId :
BFB347

m/z	Abundance
36.00	861.0
37.00	4625.0
38.00	4359.0
39.00	1759.0
39.90	293.0
44.00	993.0
45.00	768.0
46.00	130.0
47.00	883.0
47.90	732.0
49.00	4333.0
50.00	19944.0
51.00	6060.0
52.00	259.0
52.90	213.0
53.80	111.0
55.10	280.0
56.00	1794.0
57.00	2964.0
58.00	141.0
59.90	1006.0
61.00	5769.0
62.00	6250.0
63.00	5073.0
64.00	970.0
65.00	1336.0
66.00	165.0
67.00	309.0
68.00	11423.0
69.00	11578.0
70.00	895.0
72.00	673.0
73.00	5267.0
74.00	20328.0
75.00	59528.0
76.00	5311.0
77.00	797.0
77.90	453.0
78.90	4845.0
79.90	1377.0
80.90	4819.0
81.90	1073.0
85.80	135.0
86.90	4879.0
88.00	4452.0
90.90	554.0
92.00	3685.0
93.00	5977.0
94.00	14621.0
95.00	123536.0
96.00	8201.0
97.10	259.0
103.80	484.0
104.80	143.0
105.80	543.0
106.70	112.0
108.10	107.0
110.90	150.0
113.00	108.0
114.90	178.0
115.80	507.0
116.90	1027.0
117.80	519.0
118.80	707.0
127.90	505.0
128.70	258.0
129.90	526.0
130.80	233.0
134.90	230.0
136.80	207.0
140.80	1140.0
141.90	256.0
142.90	2075.0
144.00	154.0
144.80	995.0
145.80	327.0
147.70	315.0
149.90	131.0
153.70	133.0
154.70	234.0
156.80	276.0
158.90	182.0
160.90	129.0
170.80	350.0
171.90	2364.0
172.90	1589.0
173.90	123008.0
174.90	8814.0
175.90	117328.0
176.90	7836.0
177.90	279.0

Instrument :
MSVOA_V
ClientSampleId :
BFB347

m/z	Abundance
36.00	786.0
37.00	4177.0
38.00	4059.0
39.00	1701.0
39.90	207.0
44.00	887.0
45.00	738.0
46.00	144.0
47.00	948.0
47.90	688.0
49.00	4107.0
50.00	18688.0
51.00	5808.0
52.00	245.0
52.90	198.0
53.80	106.0
55.10	284.0
56.00	1679.0
57.00	2834.0
57.90	111.0
59.90	1030.0
61.00	5534.0
62.00	5991.0
63.00	4869.0
64.00	897.0
65.00	1456.0
65.90	166.0
67.00	256.0
68.00	10879.0
69.00	11293.0
70.00	812.0
72.00	672.0
73.00	5019.0
74.00	19552.0
75.00	57696.0
76.00	5141.0
77.00	702.0
77.90	482.0
78.90	4647.0
79.90	1224.0
80.90	4639.0
81.90	966.0
82.90	111.0
85.80	165.0
87.00	4574.0
88.00	4360.0
91.00	554.0
92.00	3629.0
93.00	5528.0
94.00	14177.0
95.00	119752.0
96.00	7880.0
97.00	230.0
103.80	519.0
104.80	130.0
105.80	552.0
106.70	123.0
107.90	122.0
110.90	132.0
111.90	105.0
112.90	116.0
114.90	176.0
115.80	538.0
116.90	974.0
117.80	501.0
118.80	641.0
123.80	125.0
127.90	464.0
128.70	280.0
129.90	478.0
130.80	230.0
134.90	216.0
136.80	216.0
140.90	1095.0
141.80	239.0
142.90	1855.0
143.90	133.0
144.80	971.0
145.80	300.0
147.80	299.0
149.90	107.0
152.80	105.0
153.80	117.0
154.80	216.0
156.80	268.0
158.90	177.0
160.90	139.0
170.90	352.0
171.90	2380.0
172.90	1535.0
173.90	121112.0
174.90	8470.0

Instrument :
MSVOA_V
ClientSampleId :
BFB347

175.90	116136.0
176.90	7528.0
177.80	263.0

Instrument :
MSVOA_V
ClientSampleId :
BFB347