




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072624\
 Data File : VV036709.D
 Acq On : 25 Jul 2024 15:49
 Operator : SY/MD
 Sample : P3328-02
 Misc : 8.89g/10mL/MSVOA_V/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1ZT2

Manual IntegrationsAPPROVED

Quant Time: Jul 26 05:02:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 00:49:57 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/26/2024
 Supervised By :Mahesh Dadoda 07/26/2024

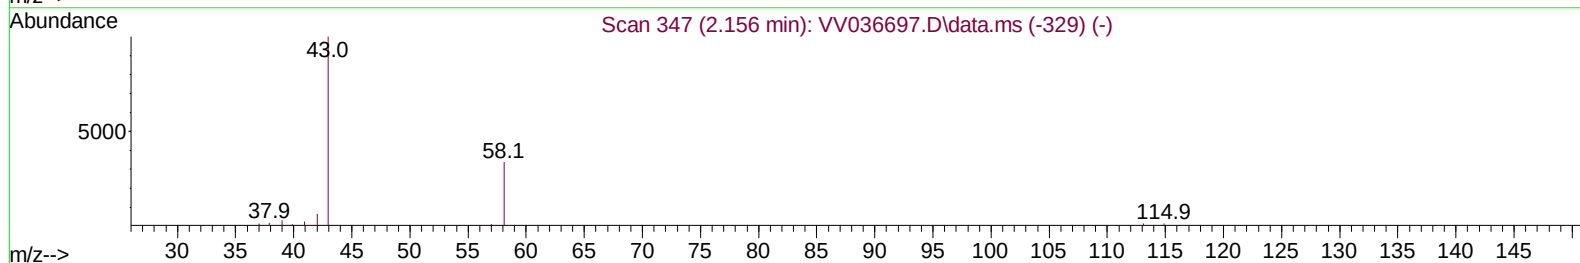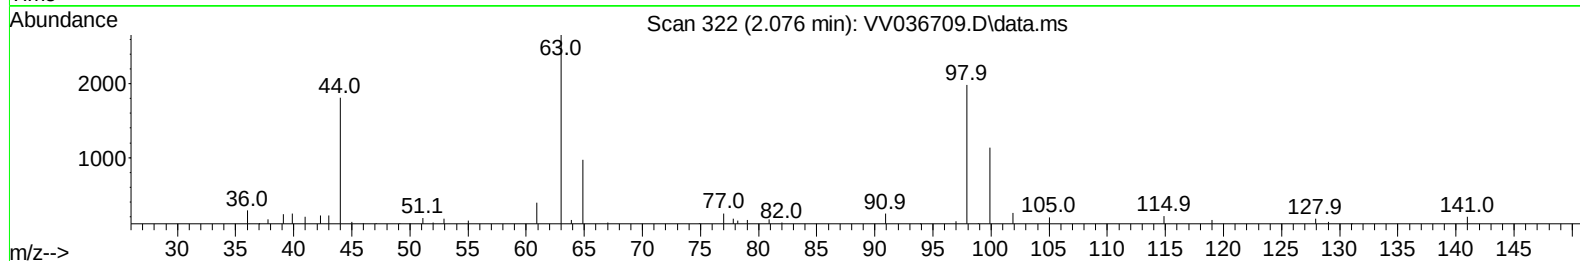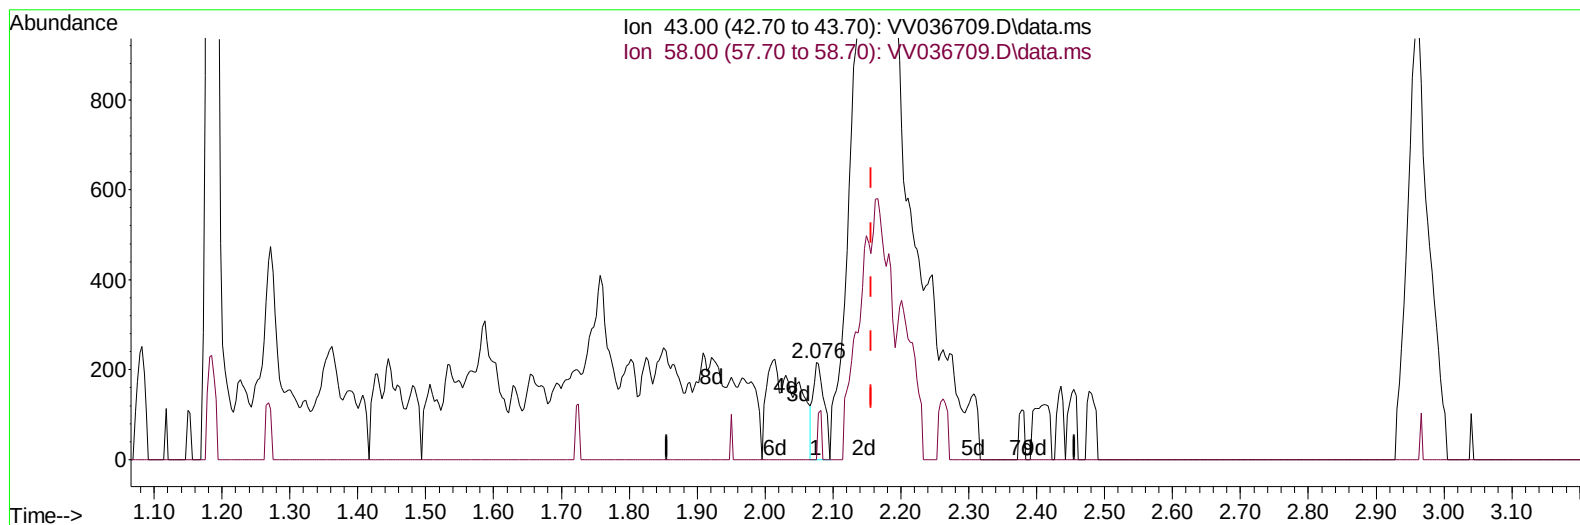

TIC: VV036709.D\data.ms

(13) Acetone (T)

2.076min (-0.080) 0.12 ug/L

response 244

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	11.50	16.80
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072624\
Data File : VV036709.D
Acq On : 25 Jul 2024 15:49
Operator : SY/MD
Sample : P3328-02
Misc : 8.89g/10mL/MSVOA_V/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1ZT2

Manual IntegrationsAPPROVED

Quant Time: Jul 26 05:02:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 00:49:57 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/26/2024
Supervised By :Mahesh Dadoda 07/26/2024

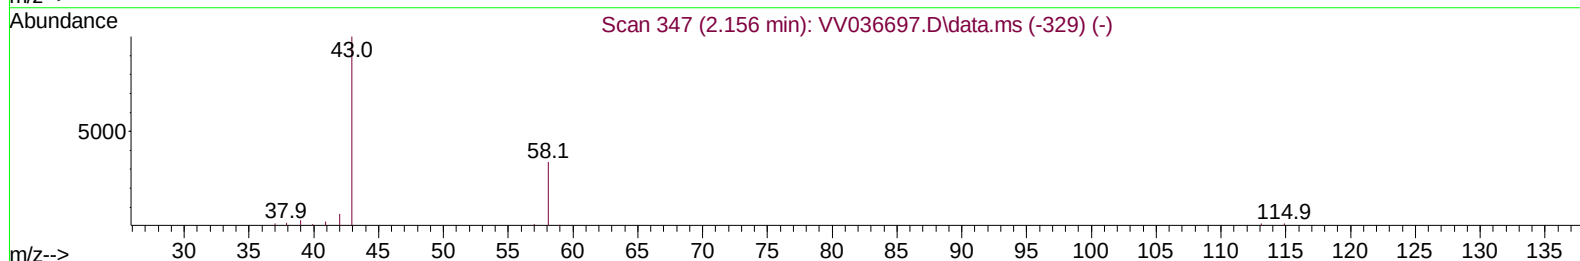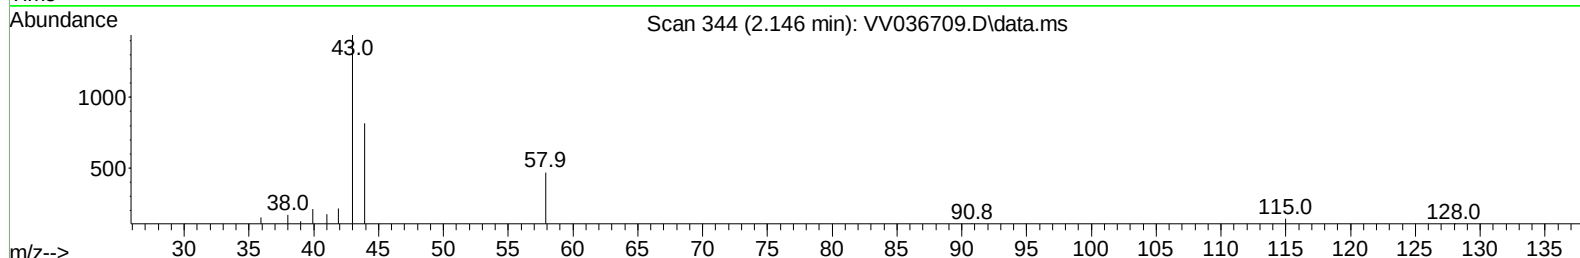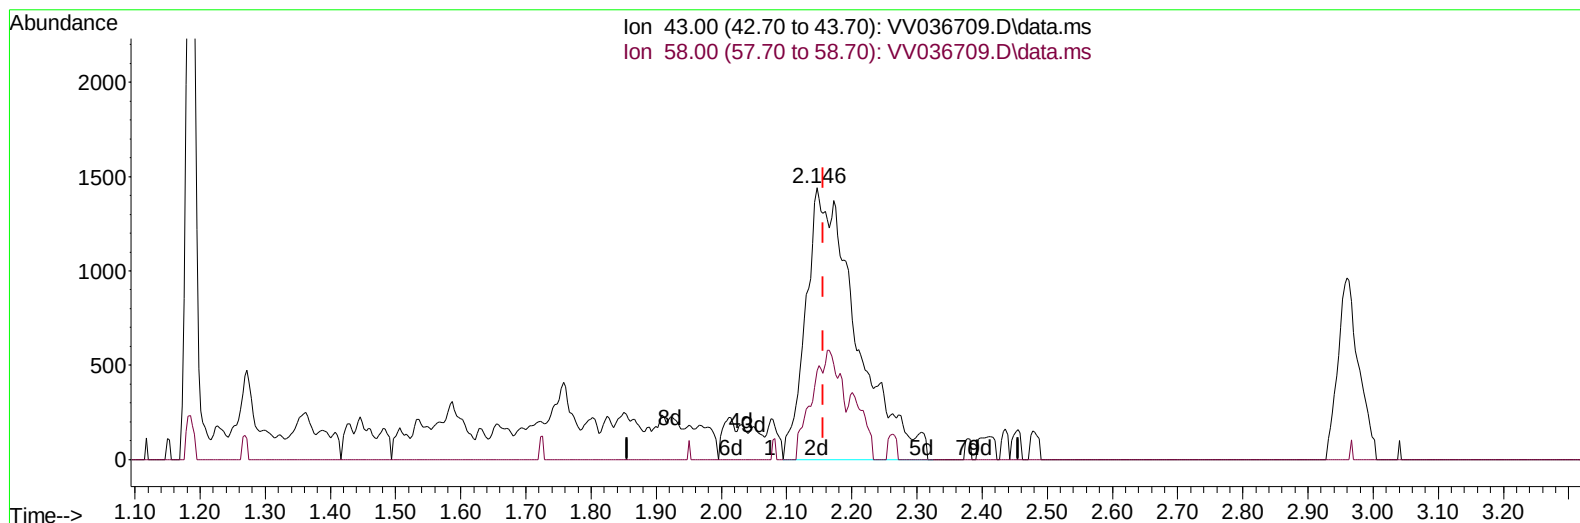

TIC: VV036709.D\data.ms

(13) Acetone (T)

2.146min (-0.010) 3.82 ug/L m

response 7755

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	11.50	0.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072624\
 Data File : VV036709.D
 Acq On : 25 Jul 2024 15:49
 Operator : SY/MD
 Sample : P3328-02
 Misc : 8.89g/10mL/MSVOA_V/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1ZT2

Manual IntegrationsAPPROVED

Quant Time: Jul 26 05:02:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 00:49:57 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/26/2024
 Supervised By :Mahesh Dadoda 07/26/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	488556	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	431544	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	148022	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	59714	11.160	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	44.640%	
7) Chloroethane-d5	1.526	69	67928	14.055	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	56.240%	
11) 1,1-Dichloroethene-d2	2.050	65	27907	9.864	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	39.440%#	
21) 2-Butanone-d5	3.834	46	53161	42.570	ug/L	-0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	85.140%	
24) Chloroform-d	4.243	84	230264	17.821	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	71.280%	
26) 1,2-Dichloroethane-d4	4.937	65	124178	19.481	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	77.920%	
32) Benzene-d6	4.953	84	324148	15.849	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	63.400%	
36) 1,2-Dichloropropane-d6	5.985	67	118864	20.396	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	81.600%	
41) Toluene-d8	7.243	98	244431	12.523	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	50.080%	
43) trans-1,3-Dichloroprop...	7.555	79	43491	16.787	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	67.160%	
47) 2-Hexanone-d5	8.030	63	38192	49.244	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.480%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	138164	27.201	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	108.800%	
66) 1,2-Dichlorobenzene-d4	11.558	152	133820	25.898	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	103.600%	
Target Compounds						
5) vinyl chloride	1.275	62	33918	4.303	ug/L	96
13) Acetone	2.146	43	7755m	3.823	ug/L	
14) Carbon disulfide	2.230	76	11362	0.543	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072624\
Data File : VV036709.D
Acq On : 25 Jul 2024 15:49
Operator : SY/MD
Sample : P3328-02
Misc : 8.89g/10mL/MSVOA_V/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1ZT2

Manual IntegrationsAPPROVED

Quant Time: Jul 26 05:02:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 00:49:57 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/26/2024
Supervised By :Mahesh Dadoda 07/26/2024

