

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072624\
 Data File : VW036700.D
 Acq On : 25 Jul 2024 12:22
 Operator : SY/MD
 Sample : P3276-18
 Misc : 7.56g/10mL/MSVOA_V/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20J7

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 07/26/2024
 Supervised By :Mahesh Dadoda 07/26/2024

Quant Time: Jul 26 05:01:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 00:49:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	275671	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	281215	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	106782	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	31163	10.321	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	41.280%		
7) Chloroethane-d5	1.526	69	38505	14.120	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	56.480%		
11) 1,1-Dichloroethene-d2	2.050	65	16273	10.193	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	40.760%#		
21) 2-Butanone-d5	3.841	46	27590m	39.155	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	78.320%		
24) Chloroform-d	4.246	84	131139	17.987	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	71.960%		
26) 1,2-Dichloroethane-d4	4.941	65	69001	19.184	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	76.720%		
32) Benzene-d6	4.957	84	169381	12.709	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	50.840%		
36) 1,2-Dichloropropane-d6	5.986	67	64989	17.113	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	68.440%#		
41) Toluene-d8	7.243	98	128327	10.089	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	40.360%		
43) trans-1,3-Dichloroprop...	7.558	79	23910	14.163	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	56.640%		
47) 2-Hexanone-d5	8.034	63	15044	29.767	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	59.540%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	74223	22.424	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	89.680%		
66) 1,2-Dichlorobenzene-d4	11.558	152	77256	20.725	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.920%		
Target Compounds					Qvalue	
13) Acetone	2.146	43	13762	12.023	ug/L	92
14) Carbon disulfide	2.233	76	11061	0.937	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072624\
Data File : VV036700.D
Acq On : 25 Jul 2024 12:22
Operator : SY/MD
Sample : P3276-18
Misc : 7.56g/10mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
E20J7

Quant Time: Jul 26 05:01:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 00:49:57 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Romaben Patel 07/26/2024
Supervised By :Mahesh Dadoda 07/26/2024

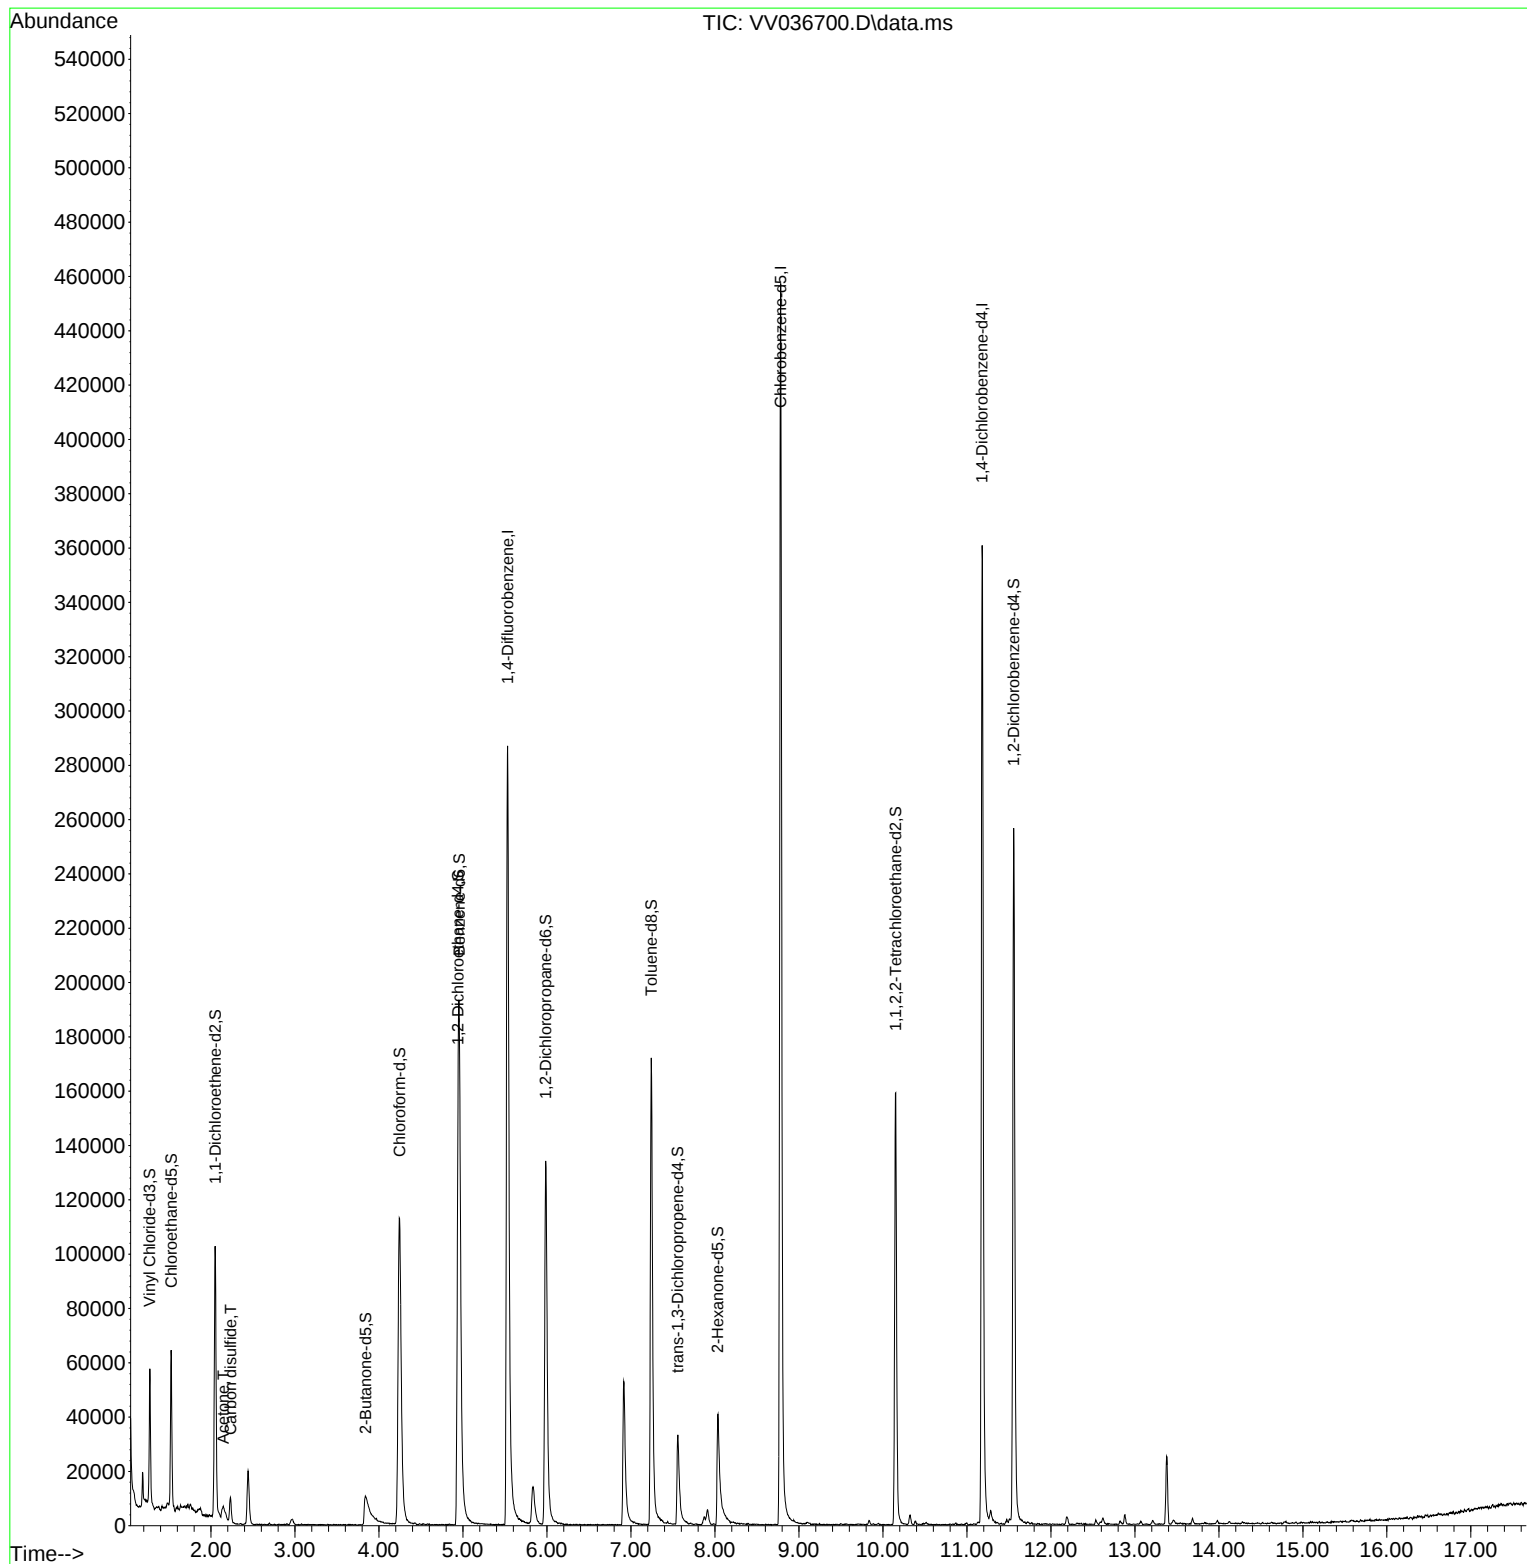

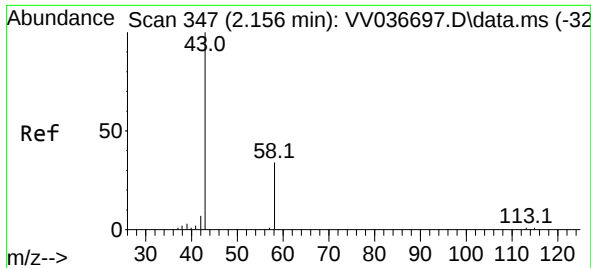

#13
Acetone
Concen: 12.023 ug/L
RT: 2.146 min Scan# 347
Delta R.T. -0.009 min
Lab File: VV036700.D
Acq: 25 Jul 2024 12:22




Instrument :
MSVOA_V
ClientSampleId :
E20J7

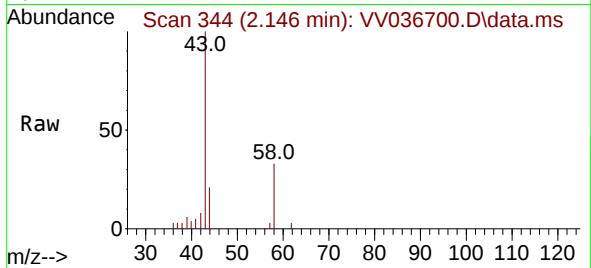

Tgt Ion: 43 Resp: 13762
Ion Ratio Lower Upper
43 100
58 14.6 0.0 23.0

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 07/26/2024
Supervised By :Mahesh Dadoda 07/26/2024

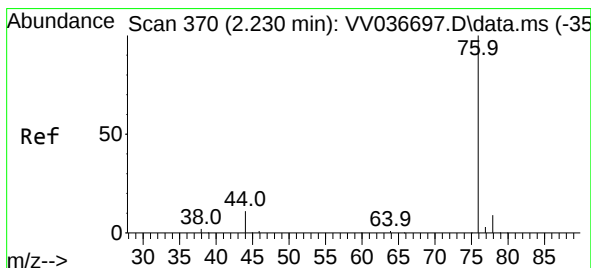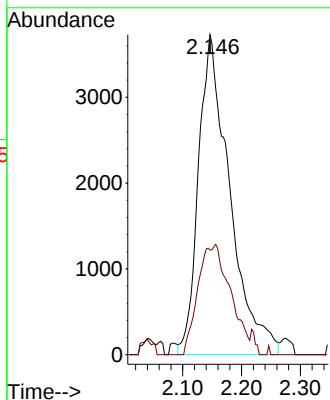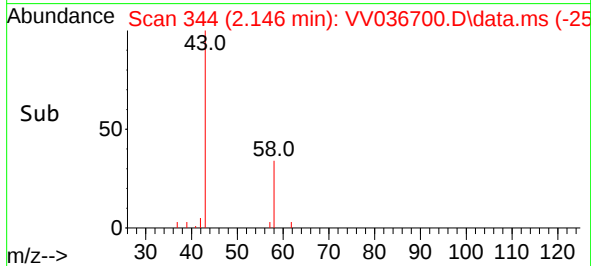

#14
Carbon disulfide
Concen: 0.937 ug/L
RT: 2.233 min Scan# 371
Delta R.T. 0.003 min
Lab File: VV036700.D
Acq: 25 Jul 2024 12:22

Tgt Ion: 76 Resp: 11061
Ion Ratio Lower Upper
76 100
78 11.0 7.5 11.3

