

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072624\
 Data File : VW036702.D
 Acq On : 25 Jul 2024 13:08
 Operator : SY/MD
 Sample : P3276-22
 Misc : 9.33g/10mL/MSVOA_V/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20J9

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 07/26/2024
 Supervised By :Mahesh Dadoda 07/26/2024

Quant Time: Jul 26 05:01:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 00:49:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	269051	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	194401	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	46040	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	44315	15.039	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.160%		
7) Chloroethane-d5	1.529	69	48680	18.290	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	73.160%		
11) 1,1-Dichloroethene-d2	2.050	65	22086	14.175	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.680%		
21) 2-Butanone-d5	3.825	46	63923m	92.951	ug/L	-0.03
Spiked Amount 50.000	Range 20 - 135		Recovery =	185.900%#		
24) Chloroform-d	4.246	84	150966	21.216	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.880%		
26) 1,2-Dichloroethane-d4	4.940	65	85340	24.310	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	97.240%		
32) Benzene-d6	4.957	84	202492	21.978	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.920%		
36) 1,2-Dichloropropane-d6	5.989	67	71935	27.401	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	109.600%		
41) Toluene-d8	7.243	98	128167	14.577	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	58.320%		
43) trans-1,3-Dichloroprop...	7.558	79	25013	21.433	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.720%		
47) 2-Hexanone-d5	8.034	63	29175	83.506	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	167.020%#		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	85088	37.187	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	148.760%#		
66) 1,2-Dichlorobenzene-d4	11.561	152	38651	24.049	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.200%		
Target Compounds						
5) Vinyl chloride	1.278	62	34165	7.870	ug/L	98
13) Acetone	2.153	43	13303	11.908	ug/L #	64
14) Carbon disulfide	2.233	76	5986	0.520	ug/L	100
16) Methylene chloride	2.442	84	32568	6.506	ug/L	95
17) trans-1,2-Dichloroethene	2.693	96	10343	2.467	ug/L	92
20) cis-1,2-Dichloroethene	3.809	96	561516	128.268	ug/L	99
34) Trichloroethene	5.838	95	5661	1.567	ug/L	93
46) Tetrachloroethene	7.911	164	1531	0.427	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072624\
Data File : VV036702.D
Acq On : 25 Jul 2024 13:08
Operator : SY/MD
Sample : P3276-22
Misc : 9.33g/10mL/MSVOA_V/SOIL/A
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
E20J9

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 07/26/2024
Supervised By :Mahesh Dadoda 07/26/2024


Quant Time: Jul 26 05:01:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 00:49:57 2024
Response via : Initial Calibration

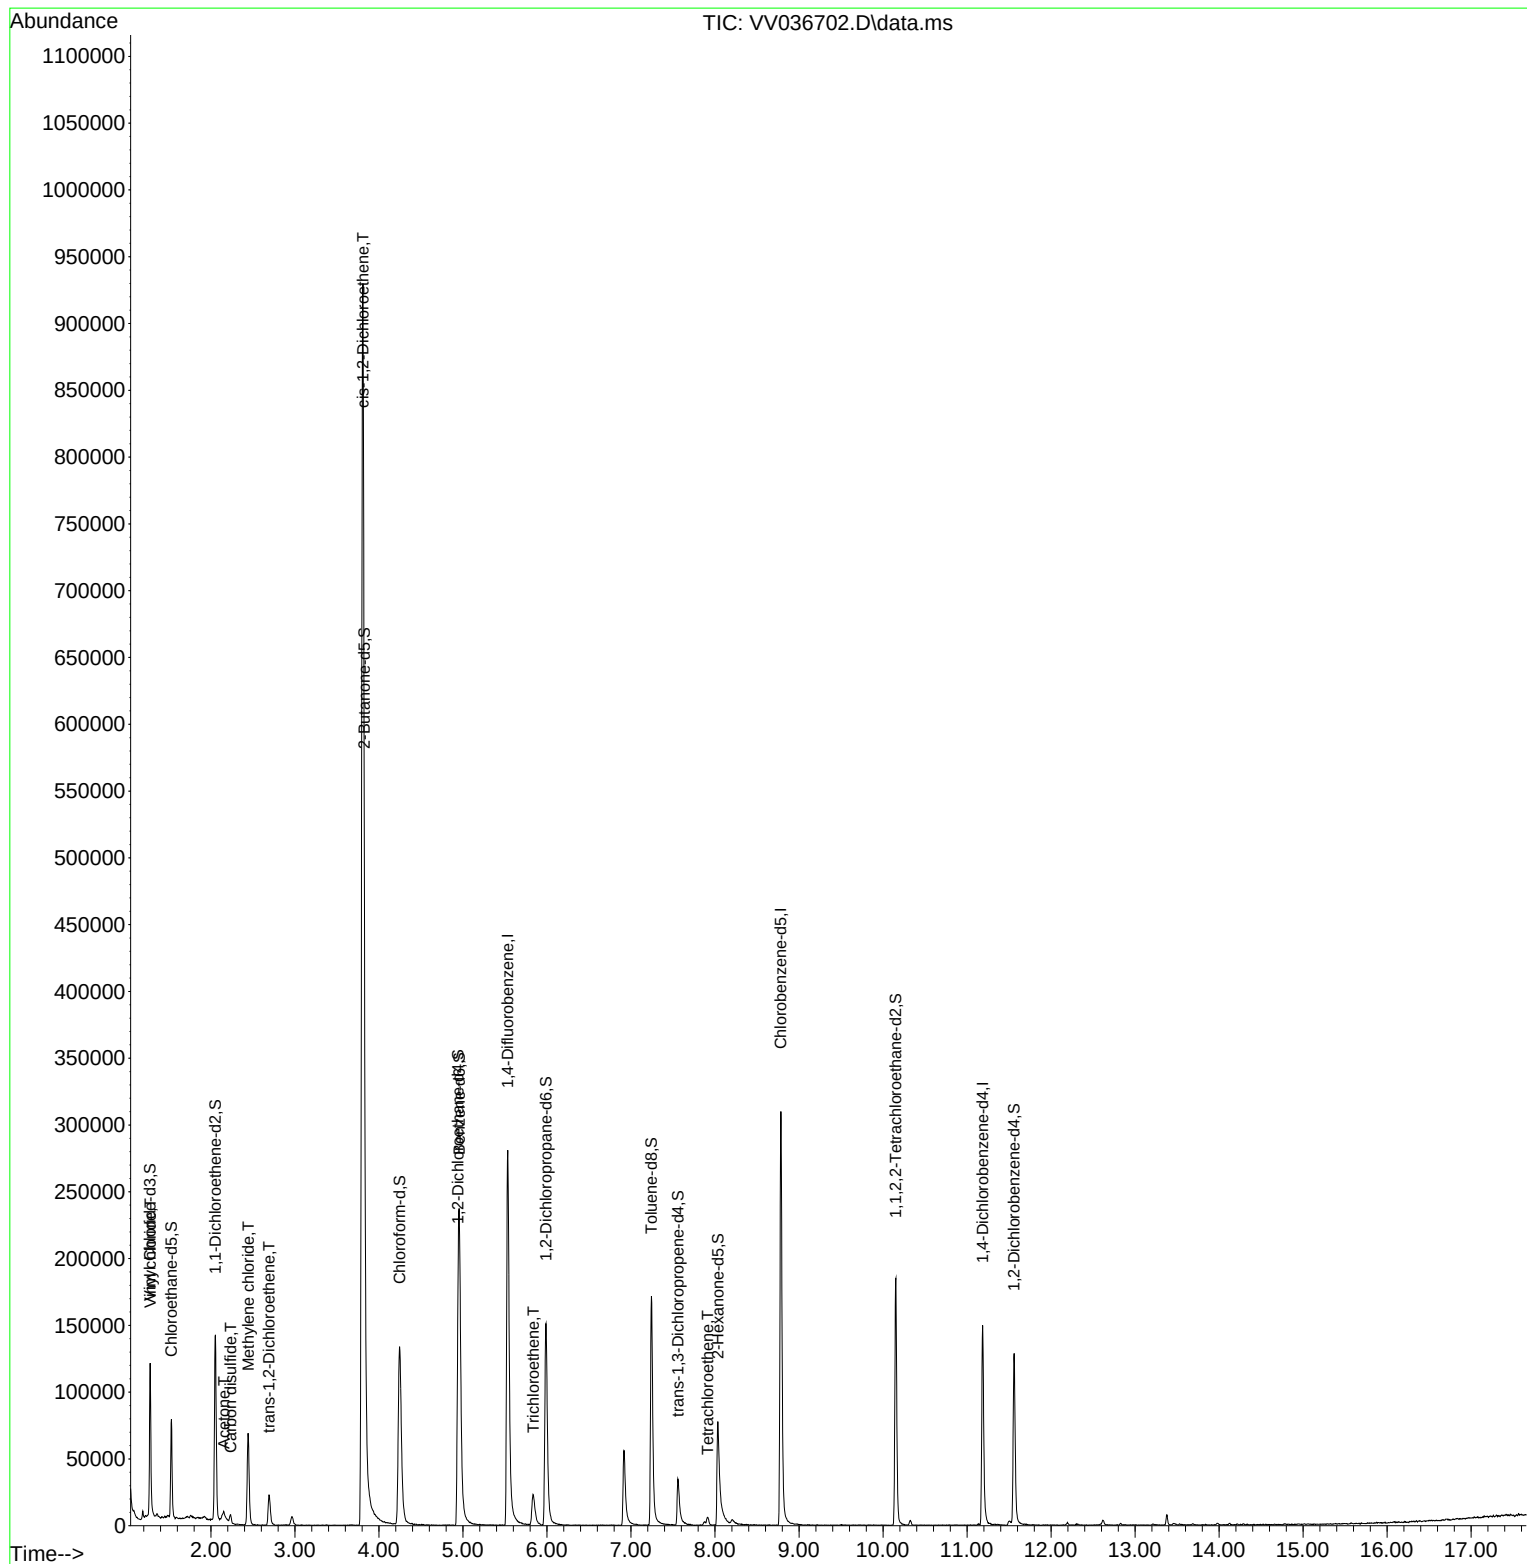

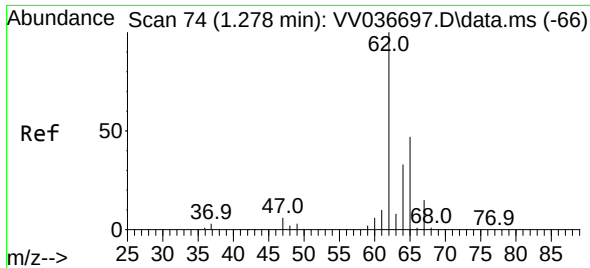

#5
 Vinyl chloride
 Concen: 7.870 ug/L
 RT: 1.278 min Scan# 74
 Delta R.T. 0.003 min
 Lab File: VV036702.D
 Acq: 25 Jul 2024 13:08




Instrument :
 MSVOA_V
 ClientSampleId :
 E20J9

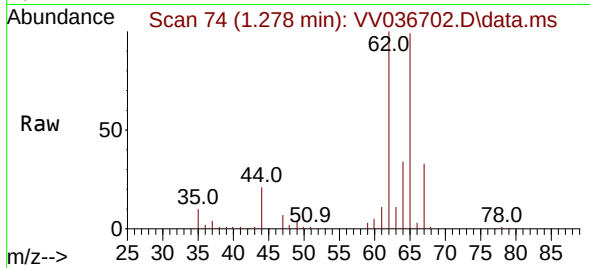

Tgt Ion: 62 Resp: 3416
 Ion Ratio Lower Upper
 62 100
 64 34.3 23.1 42.9




Manual Integrations
 APPROVED


Reviewed By :Romaben Patel 07/26/2024
 Supervised By :Mahesh Dadoda 07/26/2024

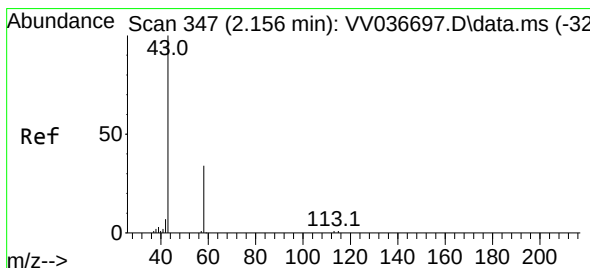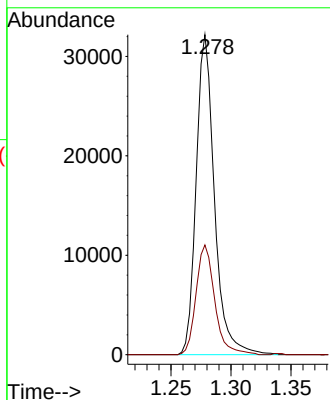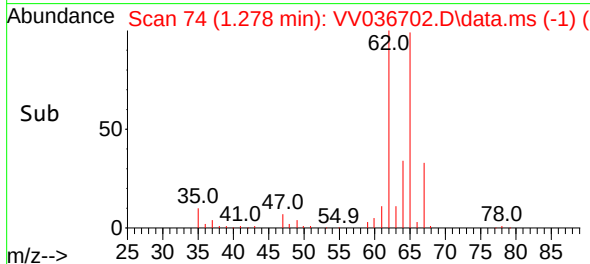

#13
 Acetone
 Concen: 11.908 ug/L
 RT: 2.153 min Scan# 346
 Delta R.T. -0.003 min
 Lab File: VV036702.D
 Acq: 25 Jul 2024 13:08


Tgt Ion: 43 Resp: 13303
 Ion Ratio Lower Upper
 43 100
 58 25.2 0.0 23.0

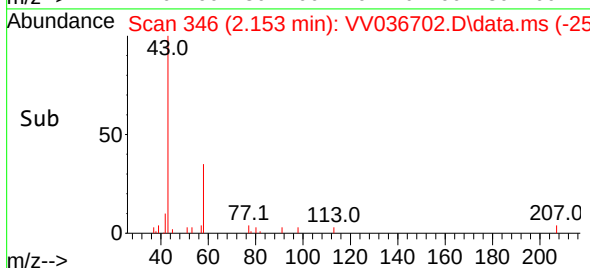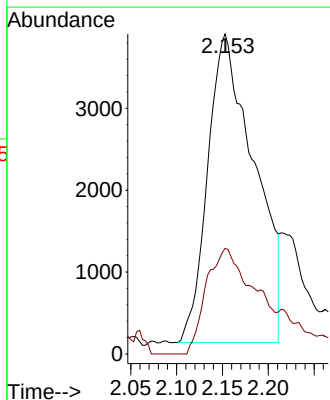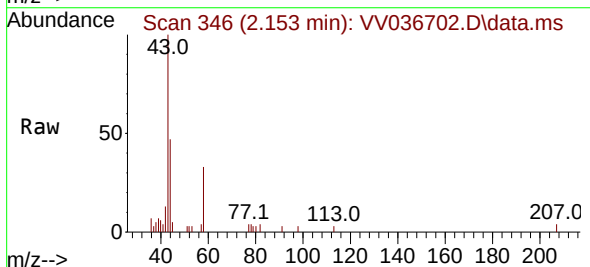

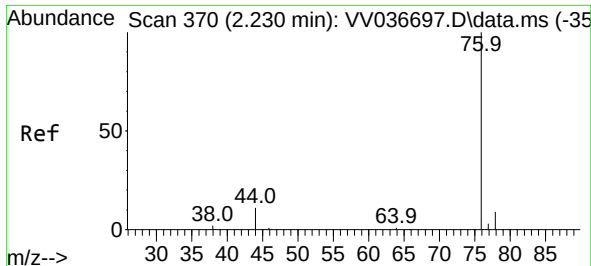

#14
Carbon disulfide
Concen: 0.520 ug/L
RT: 2.233 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV036702.D
Acq: 25 Jul 2024 13:08




Instrument :
MSVOA_V
ClientSampleId :
E20J9

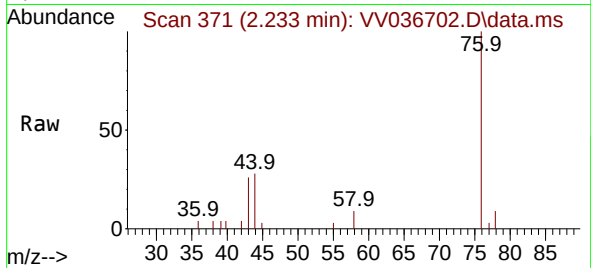

Tgt Ion: 76 Resp: 5980
Ion Ratio Lower Upper
76 100
78 9.4 7.5 11.3




Manual Integrations
APPROVED


Reviewed By :Romaben Patel 07/26/2024
Supervised By :Mahesh Dadoda 07/26/2024

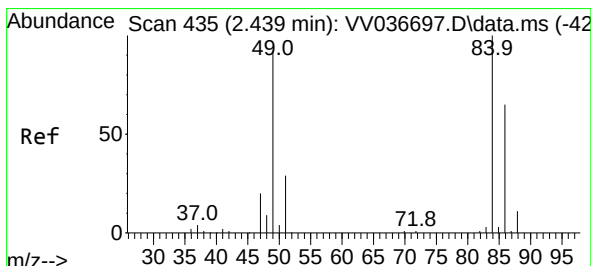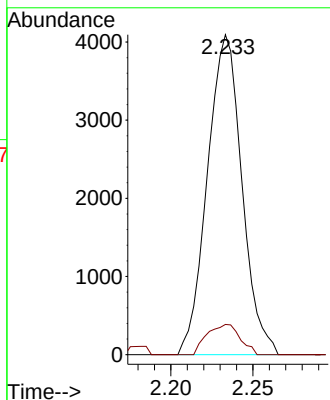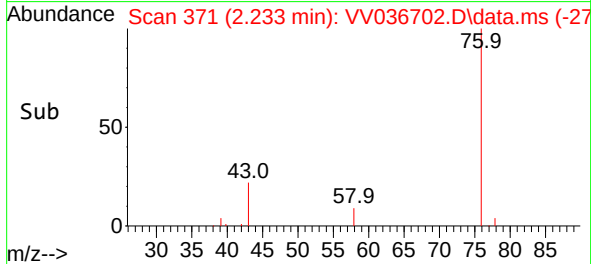

#16
Methylene chloride
Concen: 6.506 ug/L
RT: 2.442 min Scan# 436
Delta R.T. 0.003 min
Lab File: VV036702.D
Acq: 25 Jul 2024 13:08


Tgt Ion: 84 Resp: 32568
Ion Ratio Lower Upper
84 100
86 64.7 47.2 87.6
49 90.6 67.3 125.1

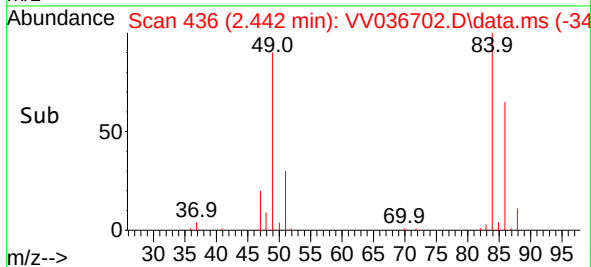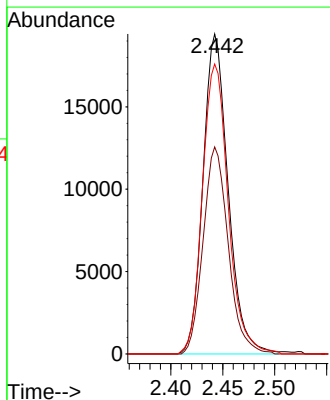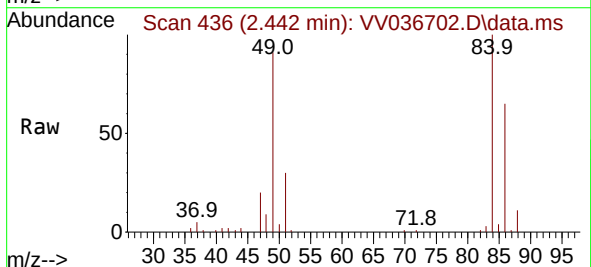

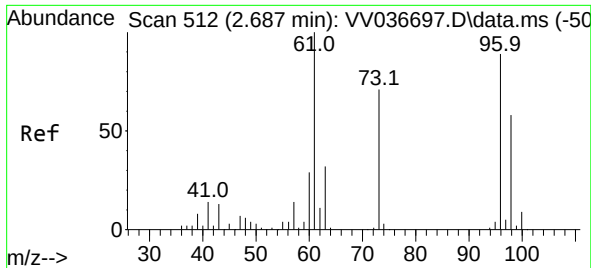

#17
trans-1,2-Dichloroethene
Concen: 2.467 ug/L
RT: 2.693 min Scan# 512
Delta R.T. 0.010 min
Lab File: VV036702.D
Acq: 25 Jul 2024 13:08




Instrument :
MSVOA_V
ClientSampleId :
E20J9

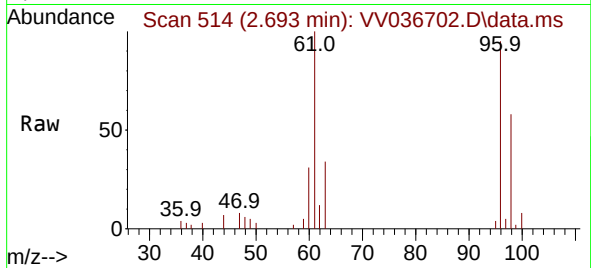

Tgt Ion: 96 Resp: 1034
Ion Ratio Lower Upper
96 100
61 104.8 81.5 151.5
98 61.2 44.3 82.3




Manual Integrations
APPROVED


Reviewed By :Romaben Patel 07/26/2024
Supervised By :Mahesh Dadoda 07/26/2024

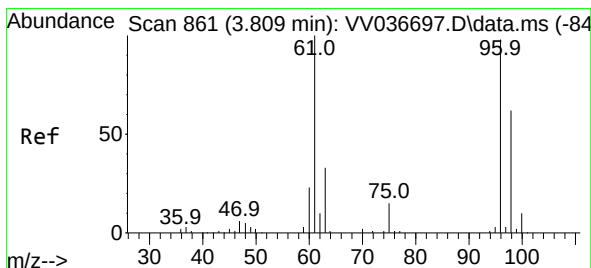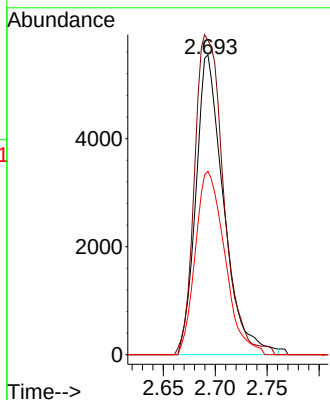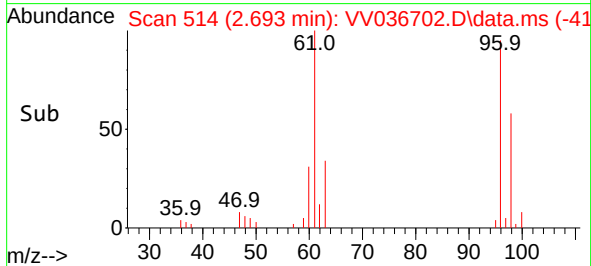

#20
cis-1,2-Dichloroethene
Concen: 128.268 ug/L
RT: 3.809 min Scan# 861
Delta R.T. 0.003 min
Lab File: VV036702.D
Acq: 25 Jul 2024 13:08


Tgt Ion: 96 Resp: 561516
Ion Ratio Lower Upper
96 100
61 103.7 73.0 135.6
98 64.7 44.8 83.2

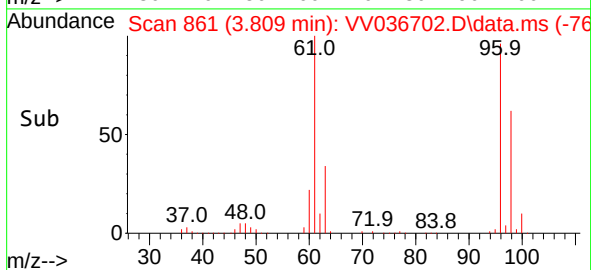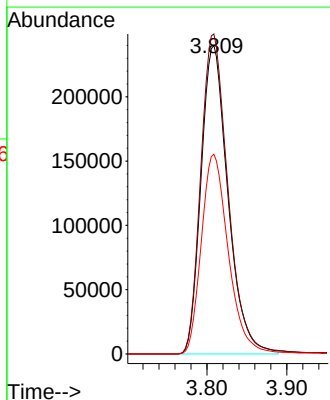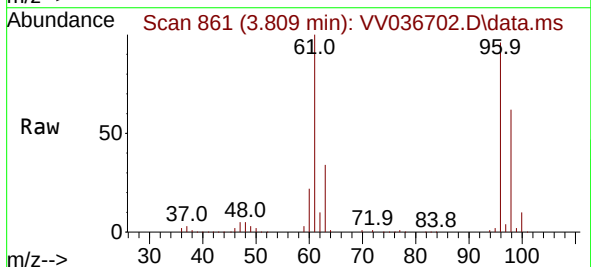

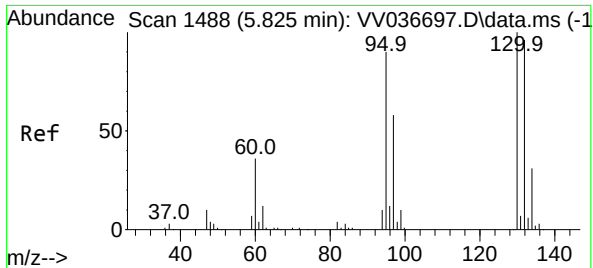

#34
Trichloroethene
Concen: 1.567 ug/L
RT: 5.838 min Scan# 1488
Delta R.T. 0.013 min
Lab File: VV036702.D
Acq: 25 Jul 2024 13:08




Instrument :
MSVOA_V
ClientSampleId :
E20J9

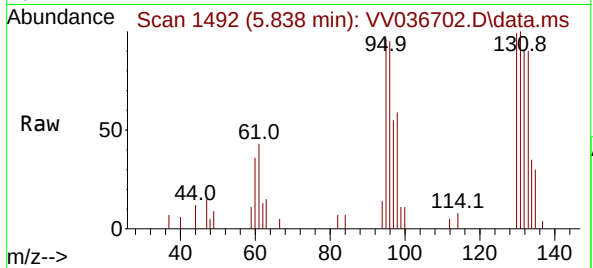


Tgt Ion: 95 Resp: 566
Ion Ratio Lower Upper
95 100
97 57.3 45.1 83.7
132 95.1 72.7 134.9
130 103.2 76.0 141.2

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 07/26/2024
Supervised By :Mahesh Dadoda 07/26/2024

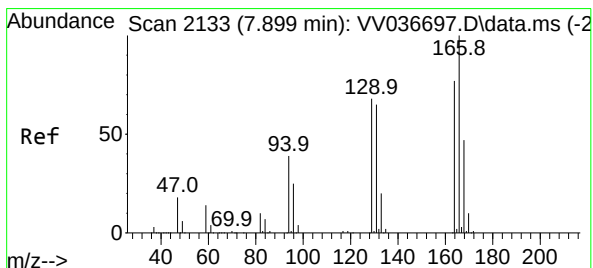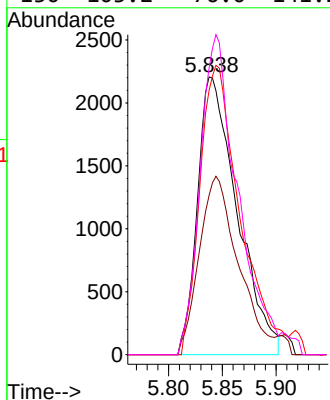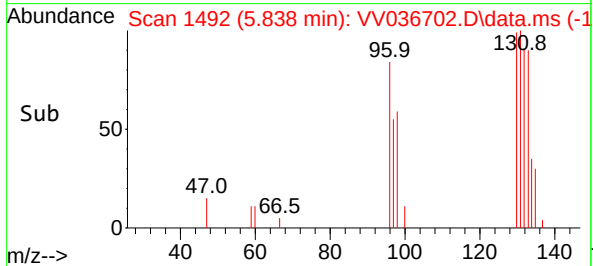

#46
Tetrachloroethene
Concen: 0.427 ug/L
RT: 7.911 min Scan# 2137
Delta R.T. 0.013 min
Lab File: VV036702.D
Acq: 25 Jul 2024 13:08

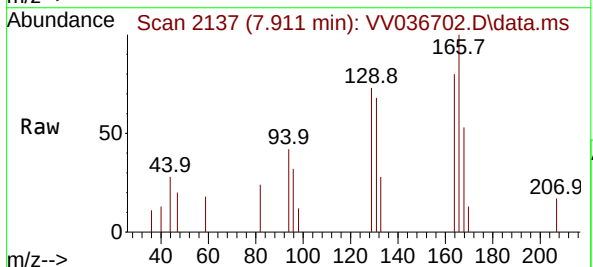

Tgt Ion:164 Resp: 1531
Ion Ratio Lower Upper
164 100
129 91.5 61.0 113.2
131 85.9 60.1 111.5
166 125.6 89.7 166.7

