

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072624\
 Data File : VW036705.D
 Acq On : 25 Jul 2024 14:17
 Operator : SY/MD
 Sample : P3276-10
 Misc : 9.79g/10mL/MSVOA_V/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20H9

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/08/2024
 Supervised By :Semsettin Yesilyurt 08/08/2024

Quant Time: Jul 26 05:01:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 00:49:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	513266	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	505503	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	201046	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	61431	10.928	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	43.720%		
7) Chloroethane-d5	1.526	69	77140	15.193	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.760%		
11) 1,1-Dichloroethene-d2	2.047	65	33447	11.253	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	45.000%		
21) 2-Butanone-d5	3.834	46	61718m	47.043	ug/L	-0.02
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.080%		
24) Chloroform-d	4.243	84	255402	18.815	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	75.240%		
26) 1,2-Dichloroethane-d4	4.937	65	139979	20.902	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	83.600%		
32) Benzene-d6	4.953	84	353737	14.765	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	59.040%		
36) 1,2-Dichloropropane-d6	5.986	67	130860	19.170	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	76.680%		
41) Toluene-d8	7.239	98	282362	12.350	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	49.400%		
43) trans-1,3-Dichloroprop...	7.551	79	52451	17.284	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	69.120%		
47) 2-Hexanone-d5	8.030	63	41622	45.815	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	91.620%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	146008	24.540	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	98.160%		
66) 1,2-Dichlorobenzene-d4	11.558	152	162005	23.084	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	92.320%		
Target Compounds						Qvalue
13) Acetone	2.169	43	13085m	6.140	ug/L	
16) Methylene chloride	2.439	84	25334	2.653	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072624\
Data File : VV036705.D
Acq On : 25 Jul 2024 14:17
Operator : SY/MD
Sample : P3276-10
Misc : 9.79g/10mL/MSVOA_V/SOIL/B
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
E20H9

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 08/08/2024
Supervised By :Semsettin Yesilyurt 08/08/2024

Quant Time: Jul 26 05:01:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 00:49:57 2024
Response via : Initial Calibration

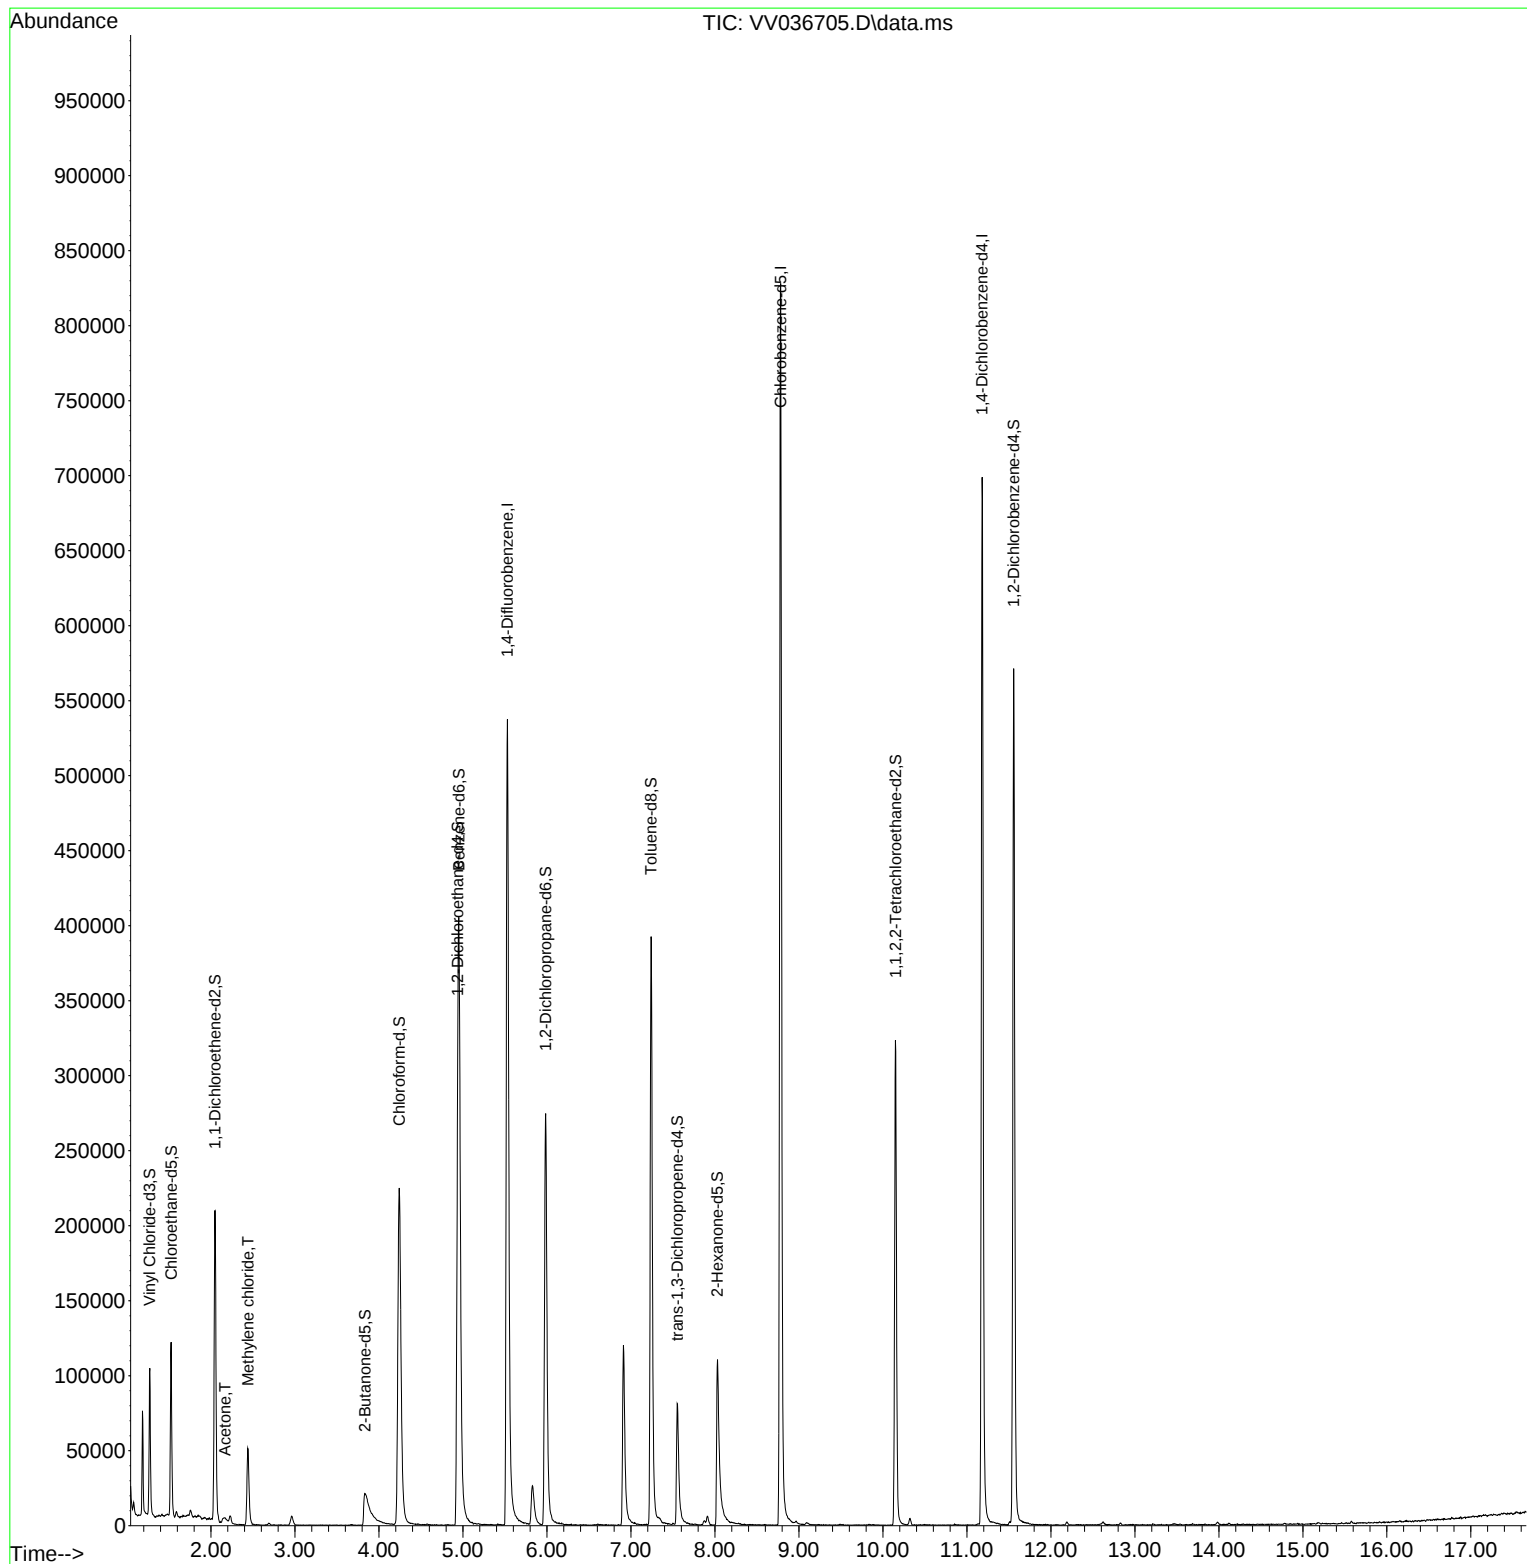

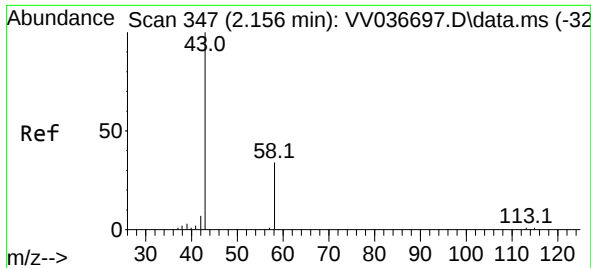

#13

Acetone

Concen: 6.140 ug/L m

RT: 2.169 min Scan# 3

Delta R.T. 0.013 min

Lab File: VV036705.D

Acq: 25 Jul 2024 14:17

Instrument :

MSVOA_V

ClientSampleId :

E20H9

Tgt Ion: 43 Resp: 1308

Ion Ratio Lower Upper

43 100





58 2.6 0.0 23.0

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 08/08/2024

Supervised By :Semsettin Yesilyurt 08/08/2024

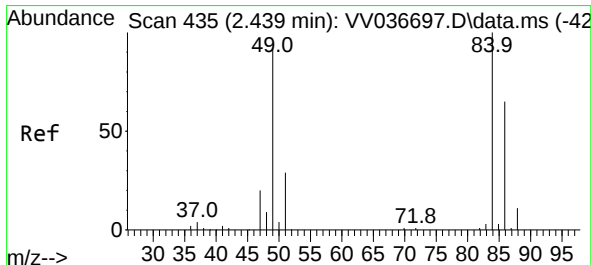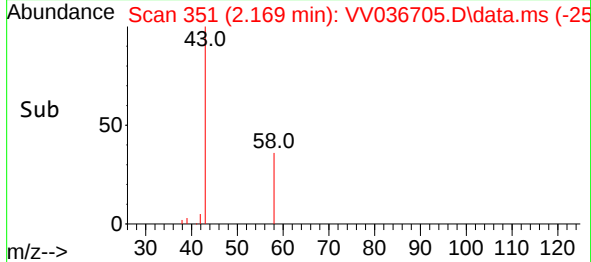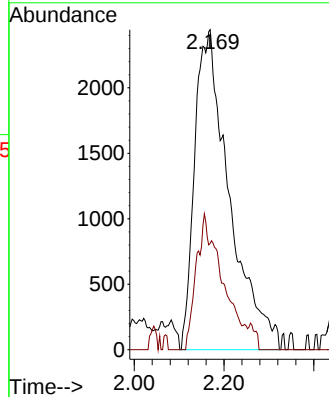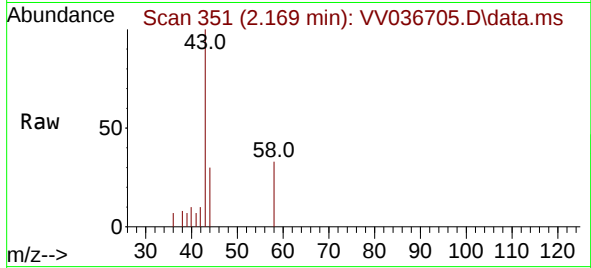

#16

Methylene chloride

Concen: 2.653 ug/L

RT: 2.439 min Scan# 435

Delta R.T. 0.000 min

Lab File: VV036705.D

Acq: 25 Jul 2024 14:17

Tgt Ion: 84 Resp: 25334

Ion Ratio Lower Upper

84 100

86 64.0 47.2 87.6

49 89.9 67.3 125.1

