

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072624\
 Data File : VW036718.D
 Acq On : 25 Jul 2024 19:28
 Operator : SY/MD
 Sample : P3328-14
 Misc : 7.45g/10mL/MSVOA_V/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L7

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 07/26/2024
 Supervised By :Mahesh Dadoda 07/26/2024

Quant Time: Jul 26 05:03:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 00:49:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	360349	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	295417	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	75032	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	43244	10.957	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	43.840%		
7) Chloroethane-d5	1.526	69	53046	14.881	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	59.520%		
11) 1,1-Dichloroethene-d2	2.050	65	22716	10.885	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	43.560%#		
21) 2-Butanone-d5	3.838	46	60198m	65.356	ug/L	-0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	130.720%		
24) Chloroform-d	4.246	84	165605	17.377	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	69.520%		
26) 1,2-Dichloroethane-d4	4.941	65	92350	19.642	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	78.560%		
32) Benzene-d6	4.957	84	229267	16.375	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	65.480%		
36) 1,2-Dichloropropane-d6	5.986	67	83888	21.028	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	84.120%		
41) Toluene-d8	7.243	98	162868	12.189	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	48.760%		
43) trans-1,3-Dichloroprop...	7.558	79	28641	16.150	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	64.600%		
47) 2-Hexanone-d5	8.030	63	33901	63.853	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	127.700%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	96632	27.791	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	111.160%		
66) 1,2-Dichlorobenzene-d4	11.561	152	54139	20.670	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.680%		
Target Compounds					Qvalue	
13) Acetone	2.156	43	28944m	19.345	ug/L	
16) Methylene chloride	2.439	84	72965	10.883	ug/L	95
34) Trichloroethene	5.841	95	10384	1.891	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072624\
Data File : VV036718.D
Acq On : 25 Jul 2024 19:28
Operator : SY/MD
Sample : P3328-14
Misc : 7.45g/10mL/MSVOA_V/SOIL/A
ALS Vial : 24 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
E20L7

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 07/26/2024
Supervised By :Mahesh Dadoda 07/26/2024

Quant Time: Jul 26 05:03:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 00:49:57 2024
Response via : Initial Calibration

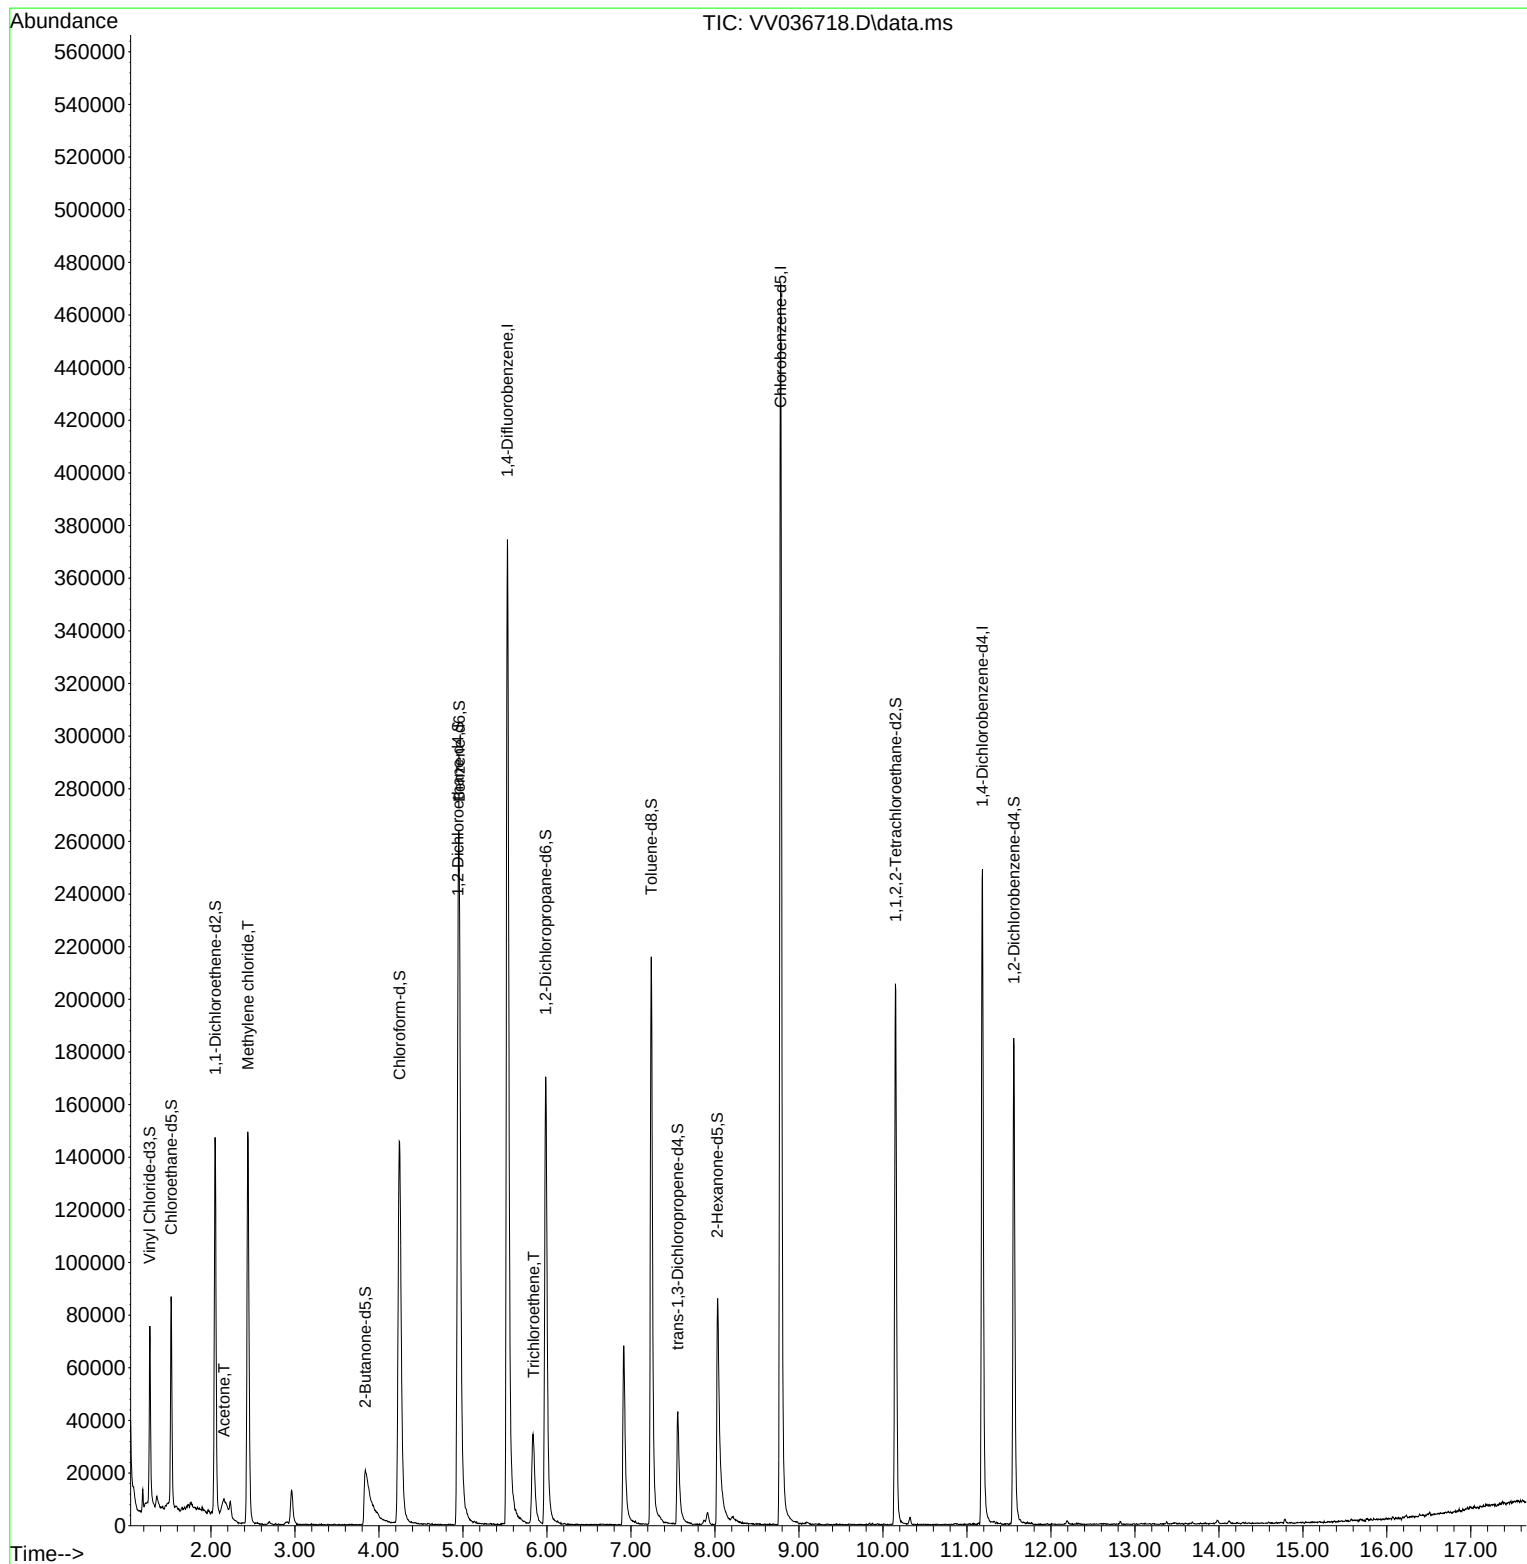

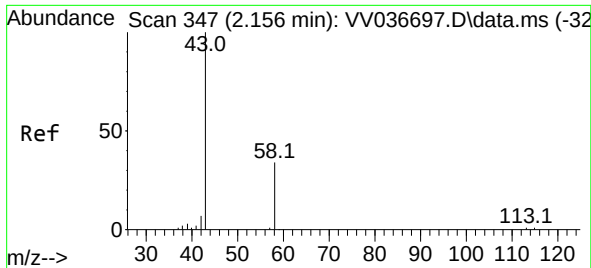

#13

Acetone

Concen: 19.345 ug/L m

RT: 2.156 min Scan# 347

Delta R.T. 0.000 min

Lab File: VV036718.D

Acq: 25 Jul 2024 19:28

Instrument :

MSVOA_V

ClientSampleId :





E20L7

Tgt Ion: 43 Resp: 28944
 Ion Ratio Lower Upper
 43 100
 58 10.6 0.0 23.0

Manual Integrations

APPROVED

Reviewed By :Romaben Patel 07/26/2024
 Supervised By :Mahesh Dadoda 07/26/2024

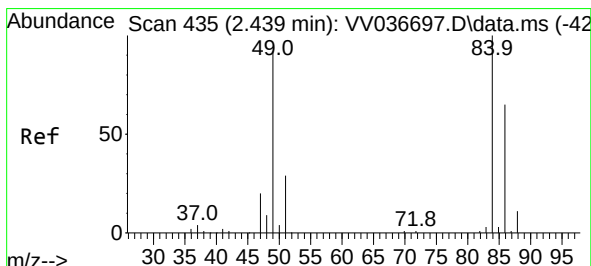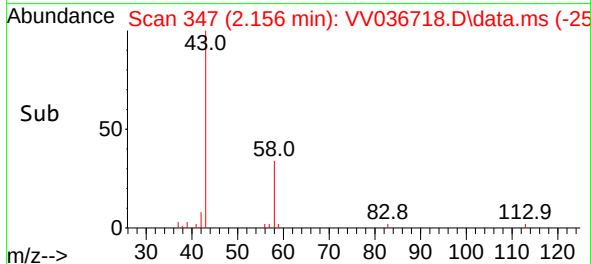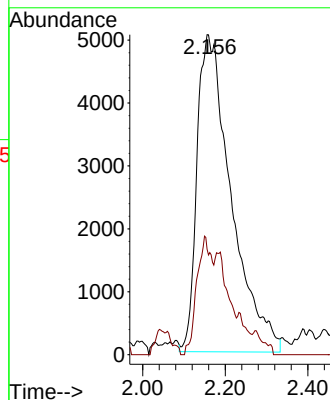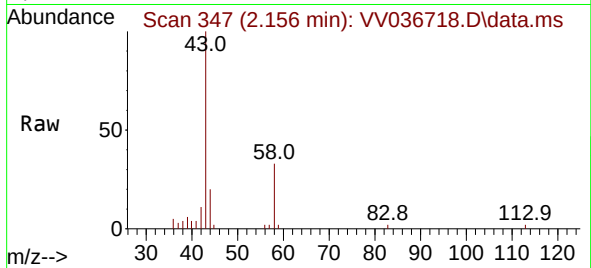

#16

Methylene chloride

Concen: 10.883 ug/L




RT: 2.439 min Scan# 435


Delta R.T. 0.000 min

Lab File: VV036718.D

Acq: 25 Jul 2024 19:28


Tgt Ion: 84 Resp: 72965
 Ion Ratio Lower Upper
 84 100
 86 64.1 47.2 87.6
 49 90.5 67.3 125.1

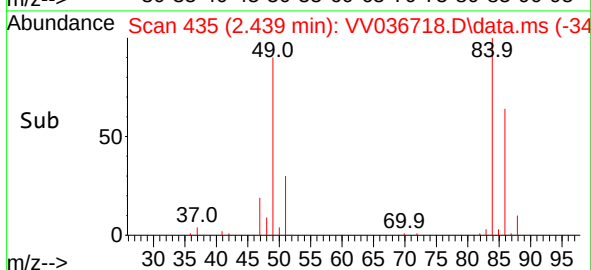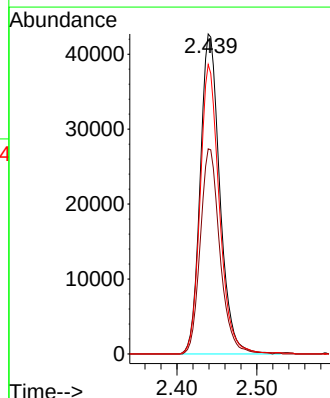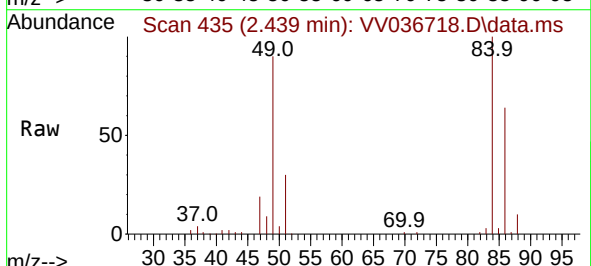

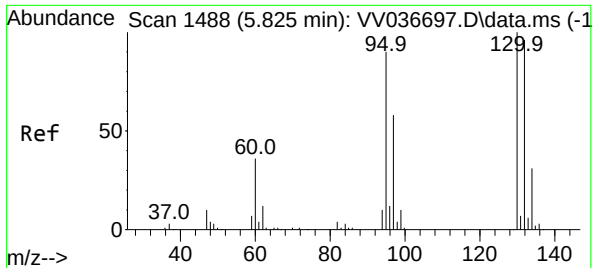

#34
 Trichloroethene
 Concen: 1.891 ug/L
 RT: 5.841 min Scan# 1488
 Delta R.T. 0.016 min
 Lab File: VV036718.D
 Acq: 25 Jul 2024 19:28

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L7

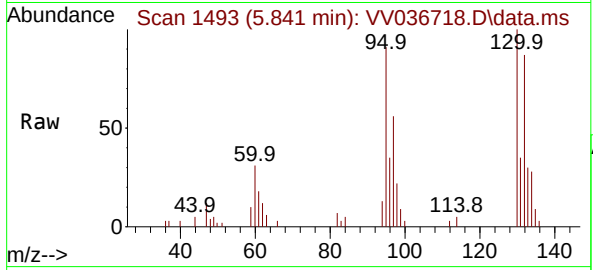

Tgt Ion: 95 Resp: 10384

Ion	Ratio	Lower	Upper
95	100		
97	62.3	45.1	83.7
132	96.3	72.7	134.9
130	110.3	76.0	141.2

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 07/26/2024
 Supervised By :Mahesh Dadoda 07/26/2024

