
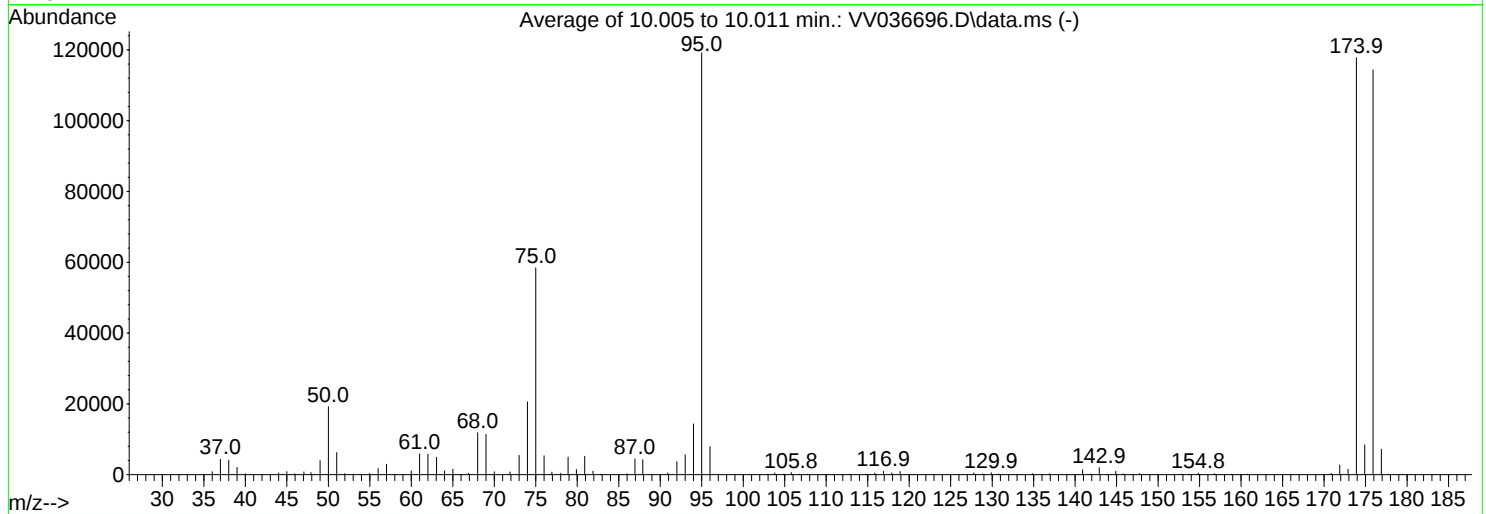


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072624\
Data File : VV036696.D
Acq On : 25 Jul 2024 09:26
Operator : SY/MD
Sample : BFB350
Misc : 5.00gM/5.00mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB350

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Title : VOC Analysis
Last Update : Sat Jul 27 04:14:21 2024

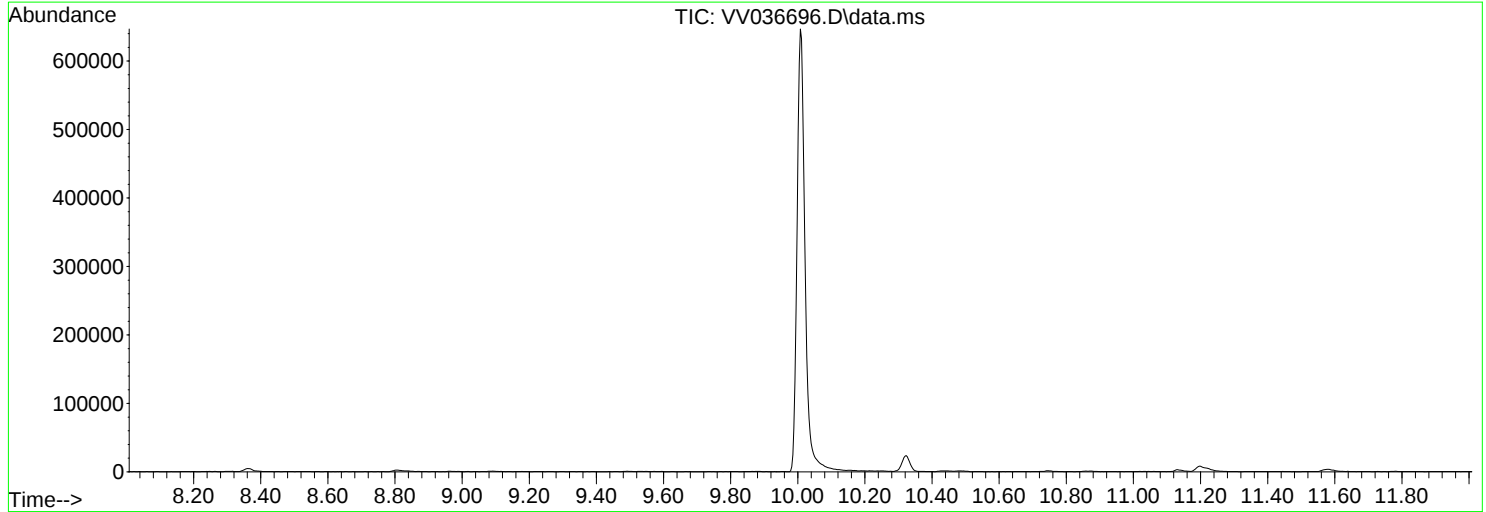

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	19208	PASS
75	95	30	80	49.0	58403	PASS
95	95	100	100	100.0	119163	PASS
96	95	5	9	6.7	7957	PASS
173	174	0.00	2	1.3	1474	PASS
174	95	50	120	98.9	117816	PASS
175	174	5	9	7.1	8398	PASS
176	174	95	101	97.1	114384	PASS
177	176	5	9	6.3	7207	PASS

m/z	Abundance
44.00	319.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

m/z	Abundance
36.00	877.0
37.00	4312.0
38.00	4101.0
39.00	2014.0
40.00	257.0
43.00	135.0
44.00	851.0
45.00	771.0
46.00	181.0
47.00	799.0
47.90	609.0
49.00	3883.0
50.00	18904.0
51.00	6102.0
51.90	276.0
53.10	192.0
53.90	141.0
54.90	385.0
56.00	1683.0
57.00	2906.0
57.90	125.0
60.00	905.0
61.00	5696.0
62.00	5905.0
63.10	4659.0
64.00	1151.0
65.00	1402.0
66.90	365.0
68.00	11738.0
69.00	11112.0
70.00	870.0
71.90	790.0
73.00	5360.0
74.00	20144.0
75.00	56936.0
76.00	5182.0
76.90	752.0
78.00	431.0
78.90	4800.0
79.90	1406.0
80.90	5132.0
81.90	994.0
82.80	119.0
86.00	245.0
86.90	4258.0
87.90	4028.0
90.90	524.0
92.00	3392.0
93.00	5306.0
94.00	14000.0
95.00	114216.0
96.00	7820.0
97.00	194.0
102.90	109.0
103.80	471.0
104.90	226.0
105.80	563.0
106.80	140.0
107.80	104.0
110.90	148.0
112.80	132.0
114.80	140.0
115.90	479.0
116.90	1018.0
117.90	476.0
118.90	889.0
127.80	544.0
128.90	177.0
129.90	476.0
130.80	162.0
134.80	227.0
136.90	207.0
140.90	1340.0
141.90	175.0
142.90	2013.0
143.90	123.0
144.90	914.0
145.80	237.0
147.70	326.0
149.90	132.0
151.90	136.0
152.90	155.0
153.70	108.0
154.90	372.0
156.80	254.0
158.90	157.0
160.80	137.0
170.80	373.0
171.90	2534.0
172.90	1393.0
173.90	109112.0
174.90	8127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

175.90	106160.0
176.90	6856.0
177.80	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

m/z	Abundance
36.00	878.0
37.00	4470.0
38.00	4222.0
39.00	2113.0
40.00	264.0
43.00	115.0
44.00	833.0
45.00	909.0
45.90	242.0
47.00	785.0
47.90	595.0
49.00	4125.0
50.00	19856.0
51.00	6428.0
51.90	302.0
53.00	204.0
53.90	152.0
54.90	362.0
56.00	1827.0
57.00	3048.0
58.00	112.0
60.00	1074.0
61.00	6112.0
62.00	5958.0
63.10	5004.0
64.00	1120.0
65.00	1613.0
66.90	416.0
68.00	12346.0
69.00	11787.0
70.00	794.0
71.90	802.0
73.00	5611.0
74.00	21280.0
75.00	60456.0
76.00	5520.0
76.90	762.0
78.00	443.0
78.90	5124.0
79.90	1543.0
80.90	5392.0
81.90	1011.0
82.80	102.0
86.00	227.0
87.00	4531.0
87.90	4464.0
90.90	532.0
92.00	3735.0
93.00	5815.0
94.00	14849.0
95.00	123208.0
96.00	8180.0
97.00	179.0
102.90	125.0
103.80	485.0
104.90	191.0
105.80	620.0
106.80	168.0
110.90	158.0
111.80	102.0
112.80	154.0
114.80	142.0
115.90	485.0
116.90	946.0
117.90	534.0
118.90	952.0
127.80	520.0
128.80	224.0
129.90	579.0
130.80	183.0
134.90	266.0
136.90	269.0
140.90	1386.0
141.80	218.0
142.90	2035.0
143.80	145.0
144.90	966.0
145.80	262.0
147.70	354.0
149.90	137.0
151.90	153.0
152.80	175.0
153.70	126.0
154.90	417.0
156.80	283.0
158.80	153.0
160.80	155.0
170.90	377.0
171.90	2792.0
172.90	1502.0
173.90	121744.0
174.90	8605.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

175.90	118240.0
176.90	7492.0
177.80	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

m/z	Abundance
36.00	761.0
37.00	4184.0
38.00	3891.0
39.00	2016.0
40.00	262.0
43.00	107.0
44.00	745.0
45.00	929.0
45.90	225.0
47.10	754.0
47.90	557.0
49.00	3974.0
50.00	18864.0
51.00	6138.0
52.00	281.0
53.00	192.0
53.90	156.0
55.00	309.0
56.00	1709.0
57.00	2927.0
58.00	117.0
60.00	1160.0
61.00	5832.0
62.00	5551.0
63.00	4940.0
64.00	957.0
65.00	1612.0
66.00	107.0
66.90	386.0
68.00	11464.0
69.00	11277.0
70.00	736.0
71.90	693.0
73.00	5289.0
74.00	20256.0
75.00	57816.0
76.00	5266.0
77.00	724.0
78.00	416.0
78.90	4941.0
79.90	1402.0
80.90	5117.0
81.90	955.0
86.00	188.0
87.00	4486.0
87.90	4301.0
90.90	503.0
92.00	3805.0
93.00	5630.0
94.00	14094.0
95.00	120064.0
96.00	7870.0
97.00	153.0
102.90	113.0
103.80	509.0
104.90	144.0
105.80	597.0
106.80	169.0
107.70	111.0
110.90	142.0
111.80	111.0
112.80	144.0
114.70	145.0
115.80	459.0
116.90	905.0
117.90	526.0
118.90	939.0
127.80	454.0
128.80	232.0
129.90	595.0
130.80	176.0
134.90	279.0
136.90	255.0
140.90	1314.0
141.80	228.0
142.90	1929.0
143.80	170.0
144.90	947.0
145.80	244.0
147.80	328.0
149.90	109.0
151.90	124.0
152.80	152.0
153.70	122.0
154.80	382.0
156.80	295.0
158.80	141.0
160.80	184.0
170.80	330.0
171.90	2801.0
172.90	1526.0
173.90	122592.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

174.90	8461.0
175.90	118752.0
176.90	7272.0
177.80	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350