


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072718\
Data File : VV006718.D
Acq On : 27 Jul 2018 09:03
Operator : SY/MD
Sample : BFB72
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB72

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Aug 01 01:43:21 2018

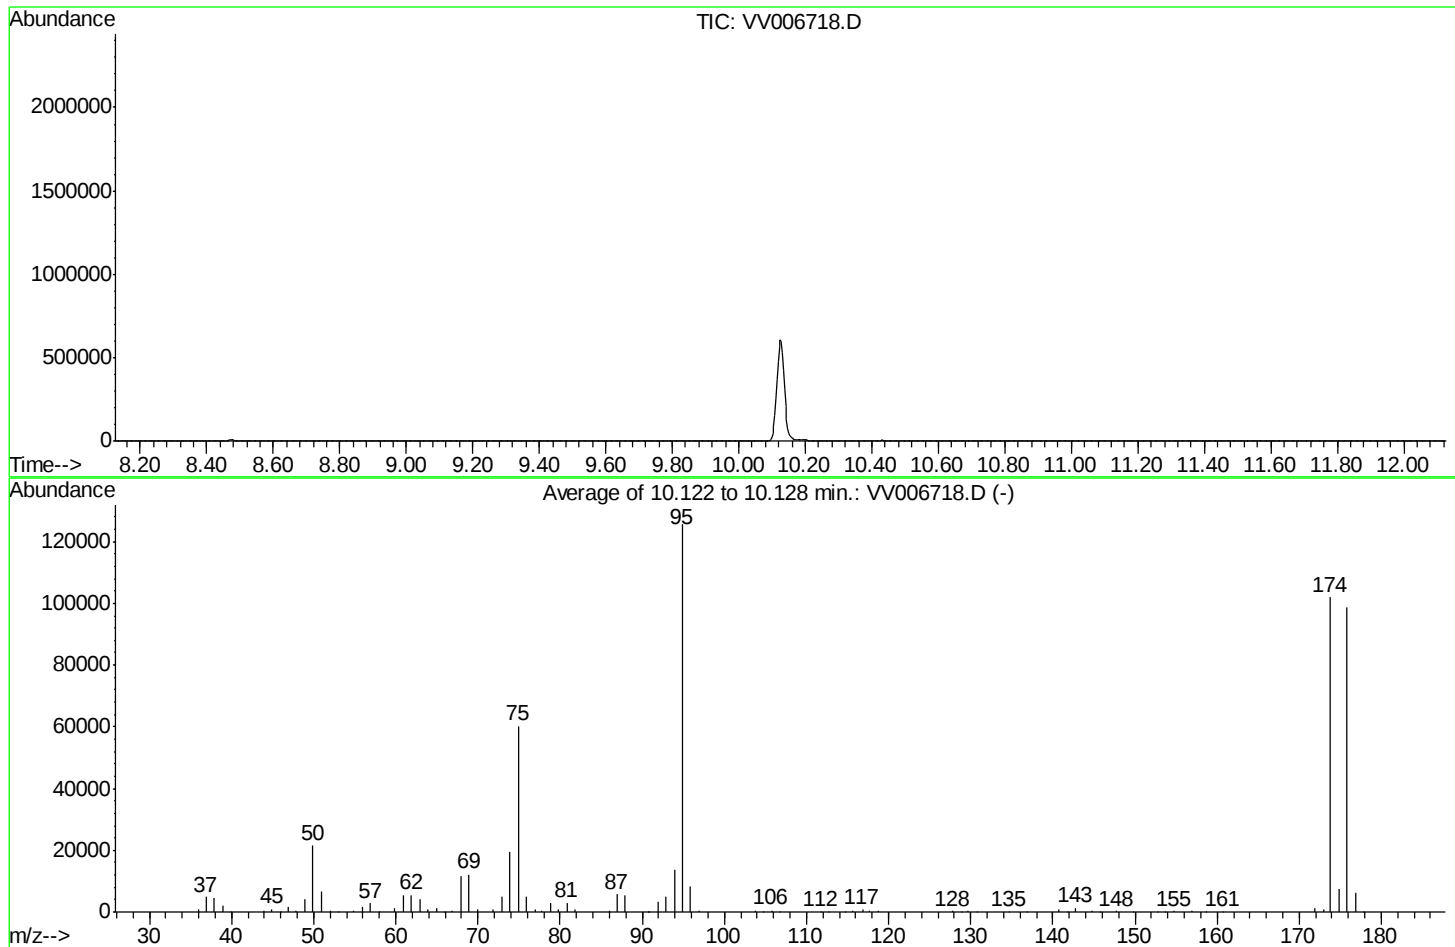

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	21469	PASS
75	95	30	80	48.0	60314	PASS
95	95	100	100	100.0	125578	PASS
96	95	5	9	6.8	8480	PASS
173	174	0.00	2	0.9	906	PASS
174	95	50	120	81.1	101816	PASS
175	174	5	9	7.1	7278	PASS
176	174	95	101	97.0	98792	PASS
177	176	5	9	6.4	6332	PASS

m/z	Abundance
35.90	983.0
36.90	4692.0
37.90	4379.0
38.90	1977.0
39.90	306.0
43.90	1118.0
44.90	930.0
46.00	110.0
46.90	1664.0
47.80	609.0
48.90	4194.0
49.90	20936.0
50.90	6449.0
52.00	329.0
53.10	116.0
54.90	324.0
55.90	1547.0
56.90	2728.0
57.90	151.0
59.90	1141.0
60.90	5211.0
61.90	5366.0
62.90	4127.0
63.90	630.0
64.90	1016.0
65.80	118.0
66.80	309.0
67.90	10881.0
68.90	11605.0
69.90	792.0
71.90	636.0
72.90	5045.0
73.90	18920.0
74.90	58264.0
76.00	4857.0
76.90	779.0
77.80	483.0
78.90	2909.0
79.80	866.0
80.80	3068.0
81.80	794.0
86.00	255.0
86.90	5568.0
87.90	5296.0
90.70	354.0
91.90	3331.0
92.90	4967.0
93.90	13159.0
94.90	121136.0
95.90	8334.0
97.10	265.0
103.80	378.0
105.80	420.0
106.80	133.0
111.80	117.0
114.80	108.0
115.70	363.0
116.80	636.0
117.70	406.0
118.80	595.0
127.90	385.0
128.80	226.0
129.70	374.0
130.80	213.0
134.70	189.0
136.80	118.0
140.80	858.0
141.80	119.0
142.80	1139.0
144.90	216.0
145.70	174.0
147.80	225.0
152.70	104.0
153.70	104.0
154.80	234.0
156.90	242.0
171.80	1147.0
172.90	817.0
173.80	95784.0
174.90	6943.0
175.80	92904.0
176.90	6005.0
177.80	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	1045.0
36.90	5016.0
37.90	4570.0
38.90	2008.0
39.90	321.0
43.90	1130.0
44.90	959.0
45.90	120.0
46.90	1721.0
47.80	650.0
48.90	4366.0
49.90	22120.0
50.90	6726.0
52.00	304.0
53.00	116.0
54.90	375.0
55.90	1617.0
56.90	2893.0
57.90	165.0
59.90	1224.0
60.90	5571.0
61.90	5759.0
62.90	4405.0
63.90	702.0
64.90	1096.0
65.90	107.0
66.80	357.0
67.90	11846.0
68.90	12589.0
69.90	872.0
71.90	723.0
72.90	5268.0
73.90	20376.0
74.90	62176.0
75.90	5142.0
76.90	807.0
77.80	561.0
78.80	3191.0
79.80	962.0
80.80	3136.0
81.80	828.0
86.00	287.0
86.90	5878.0
87.90	5509.0
90.90	346.0
91.90	3509.0
92.90	5371.0
93.90	14137.0
94.90	129720.0
95.90	8787.0
97.00	241.0
103.80	429.0
104.70	120.0
105.80	460.0
106.80	132.0
111.80	136.0
114.70	116.0
115.70	419.0
116.90	727.0
117.70	425.0
118.80	637.0
127.80	430.0
128.80	214.0
129.70	410.0
130.80	227.0
134.70	214.0
136.80	142.0
140.80	958.0
141.80	131.0
142.80	1280.0
144.90	243.0
145.70	187.0
147.80	267.0
149.70	107.0
152.70	114.0
154.80	289.0
156.90	259.0
158.70	107.0
160.70	103.0
171.90	1205.0
173.00	953.0
173.80	104976.0
174.90	7524.0
175.80	101848.0
176.90	6560.0
177.80	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	949.0
36.90	4803.0
37.90	4280.0
38.90	1861.0
39.80	326.0
43.90	1106.0
44.90	928.0
45.90	135.0
46.90	1617.0
47.80	620.0
48.90	4242.0
49.90	21352.0
50.90	6442.0
52.00	284.0
52.90	111.0
54.90	364.0
55.90	1531.0
56.90	2798.0
57.90	151.0
59.90	1115.0
60.90	5337.0
61.90	5491.0
62.90	4153.0
64.00	667.0
64.90	1102.0
65.90	106.0
66.90	334.0
67.90	11835.0
68.90	12343.0
69.90	907.0
71.90	711.0
72.90	5076.0
73.90	19816.0
74.90	60504.0
75.90	4955.0
76.90	776.0
77.80	552.0
78.80	3142.0
79.80	955.0
80.80	2960.0
81.80	750.0
85.90	282.0
86.90	5514.0
87.90	5036.0
90.90	320.0
91.90	3402.0
92.90	5213.0
93.90	13930.0
94.90	125880.0
95.90	8320.0
96.90	248.0
103.80	435.0
104.80	141.0
105.80	450.0
111.70	137.0
112.70	104.0
114.70	120.0
115.70	381.0
116.90	749.0
117.60	392.0
118.80	616.0
127.80	419.0
128.90	195.0
129.70	390.0
130.80	209.0
134.70	197.0
136.80	164.0
140.80	989.0
141.80	124.0
142.80	1342.0
144.80	241.0
145.60	158.0
147.70	296.0
149.80	124.0
152.80	105.0
154.80	308.0
156.90	238.0
158.70	119.0
160.70	109.0
171.90	1146.0
172.90	948.0
173.80	104688.0
174.90	7367.0
175.80	101624.0
176.90	6433.0
177.80	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
39.80	171.0
43.90	528.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72