

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072718\
 Data File : VV006725.D
 Acq On : 27 Jul 2018 14:11
 Operator : SY/MD
 Sample : J4148-10
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SX5

Quant Time: Jul 28 02:50:50 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 28 02:24:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	217018	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	202004	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	84636	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72207	6.39	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	127.80%
7) Chloroethane-d5	1.58	69	53850	6.07	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	121.40%
11) 1,1-Dichloroethene-d2	2.13	63	95859	4.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.60%
20) 2-Butanone-d5	3.95	46	184512	52.28	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.56%
24) Chloroform-d	4.41	84	122841	5.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.00%
26) 1,2-Dichloroethane-d4	5.09	65	62553	6.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	121.00%
32) Benzene-d6	5.10	84	255617	6.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	123.20%
36) 1,2-Dichloropropane-d6	6.12	67	81227	5.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.80%
41) Toluene-d8	7.37	98	218807	6.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.60%
43) trans-1,3-Dichloropropene-	7.67	79	25171	5.50	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	110.00%
46) 2-Hexanone-d5	8.14	63	140934	48.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.26%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	60064	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	79072	6.27	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	125.40%#


Target Compounds					Ovalue
13) Acetone	2.19	43	9502	4.232 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072718\
Data File : VV006725.D
Acq On : 27 Jul 2018 14:11
Operator : SY/MD
Sample : J4148-10
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SX5

Quant Time: Jul 28 02:50:50 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 28 02:24:46 2018
Response via : Initial Calibration

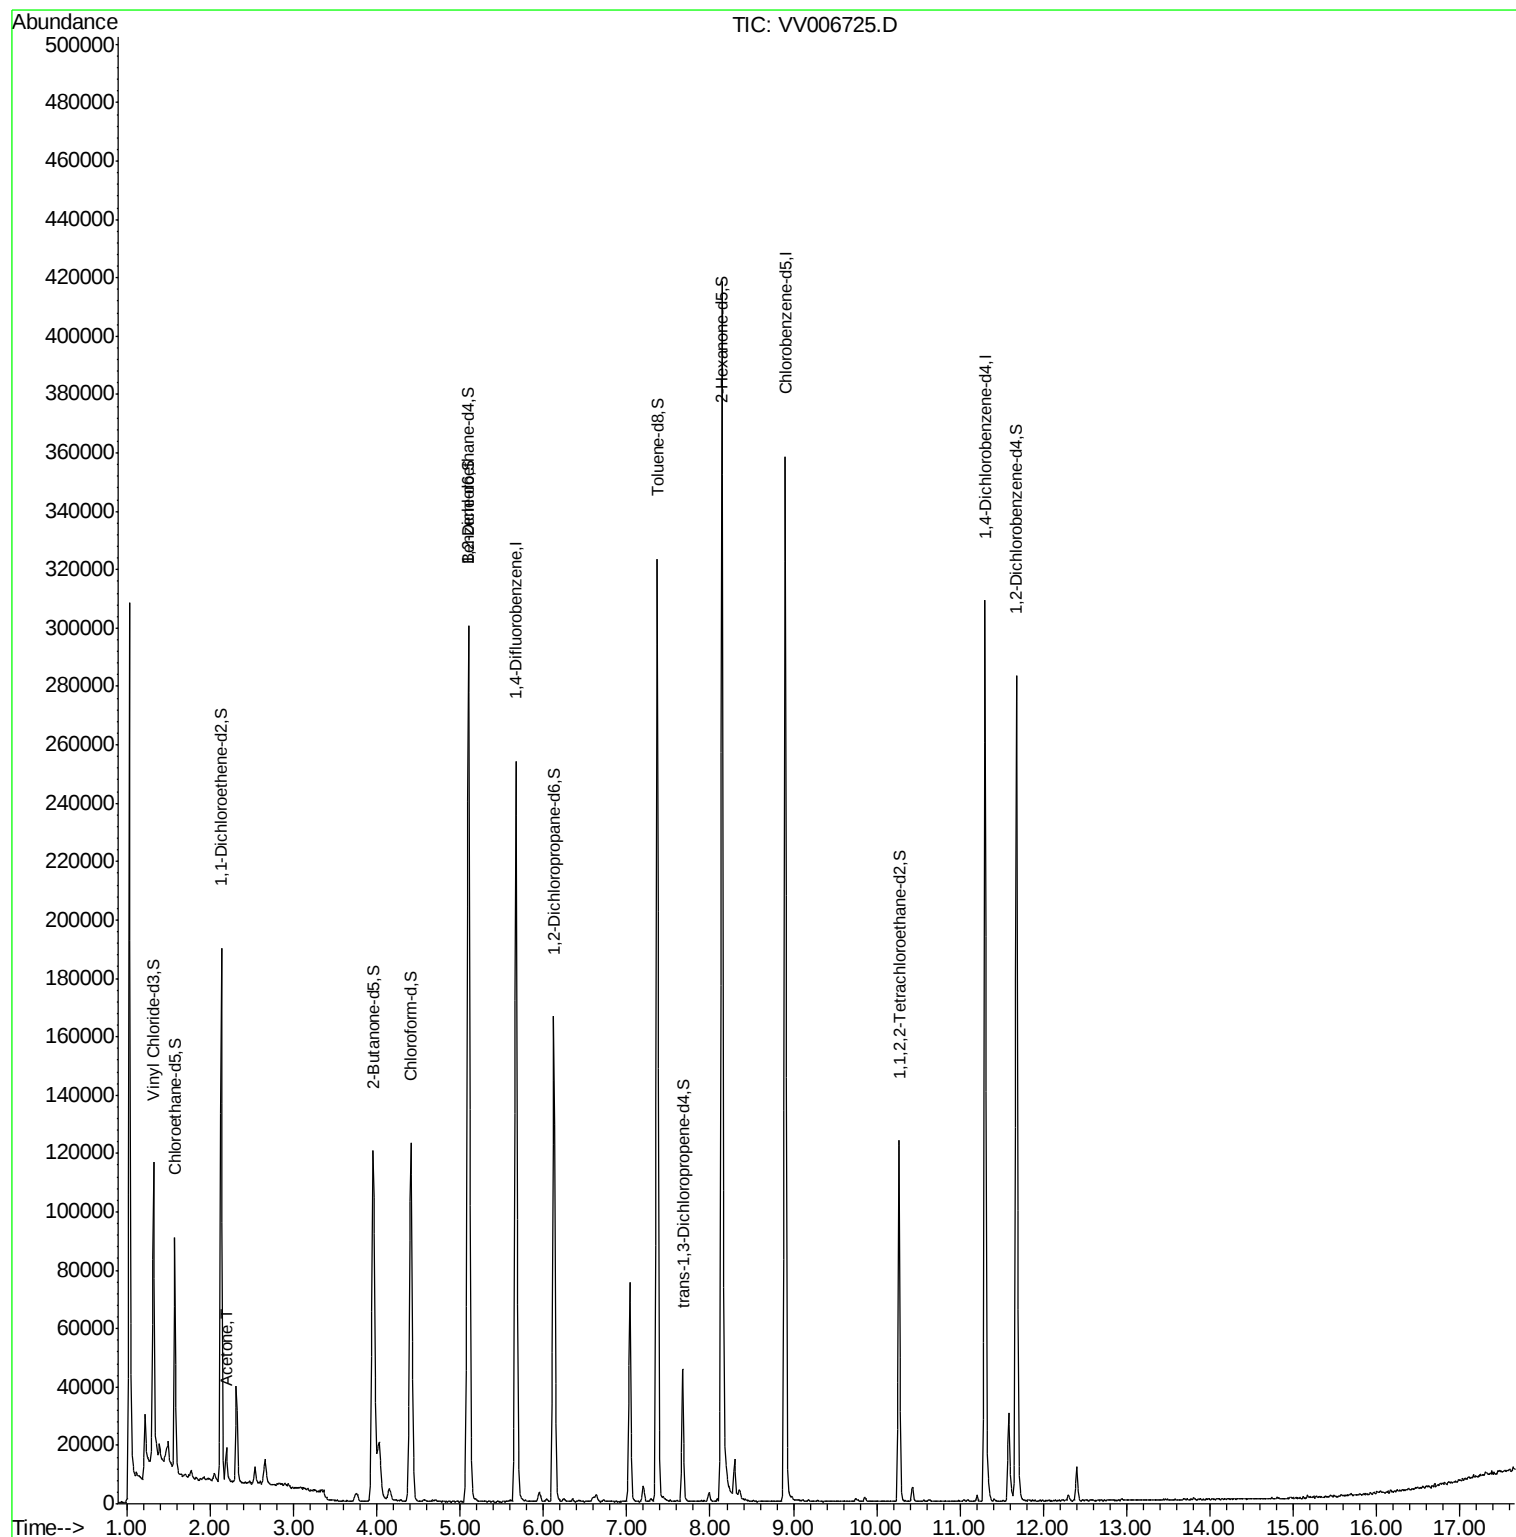

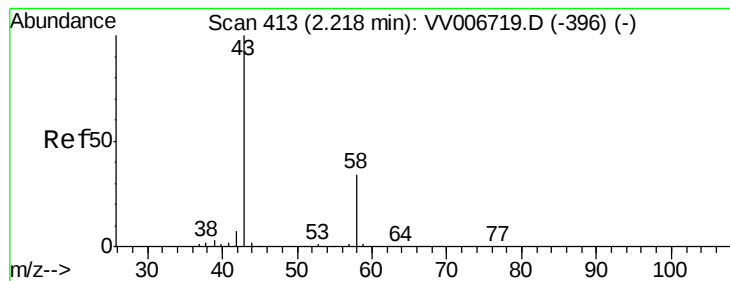

#13
Acetone
Concen: 4.232 ug/L
RT: 2.19 min Scan# 405
Delta R.T. -0.03 min
Lab File: VV006725.D
Acq: 27 Jul 2018 14:11

Instrument :
MSVOA_V
ClientSampleId :
C0SX5

Tot Ion: 43 Resp: 9502
Ion Ratio Lower Upper
43 100
58 34.9 0.0 71.4

