

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072718\
 Data File : VV006731.D
 Acq On : 27 Jul 2018 17:21
 Operator : SY/MD
 Sample : J4209-09
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC4

Quant Time: Jul 28 03:39:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 28 02:24:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	187307	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	174716	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	70509	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	59832	6.14	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	122.80%
7) Chloroethane-d5	1.58	69	48155	6.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	125.80%
11) 1,1-Dichloroethene-d2	2.13	63	82772	4.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.60%
20) 2-Butanone-d5	3.96	46	152579	50.09	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.18%
24) Chloroform-d	4.40	84	103885	5.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.60%
26) 1,2-Dichloroethane-d4	5.09	65	53754	6.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.60%
32) Benzene-d6	5.10	84	216985	6.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	120.80%
36) 1,2-Dichloropropane-d6	6.12	67	71002	5.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	117.00%
41) Toluene-d8	7.36	98	177702	5.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.20%
43) trans-1,3-Dichloropropene-	7.67	79	21350	5.39	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	107.80%
46) 2-Hexanone-d5	8.14	63	112498	44.88	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.76%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	50298	5.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	62602	5.96	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.20%


Target Compounds					Ovalue
13) Acetone	2.20	43	7749	3.999 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072718\
Data File : VV006731.D
Acq On : 27 Jul 2018 17:21
Operator : SY/MD
Sample : J4209-09
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC4

Quant Time: Jul 28 03:39:47 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 28 02:24:46 2018
Response via : Initial Calibration

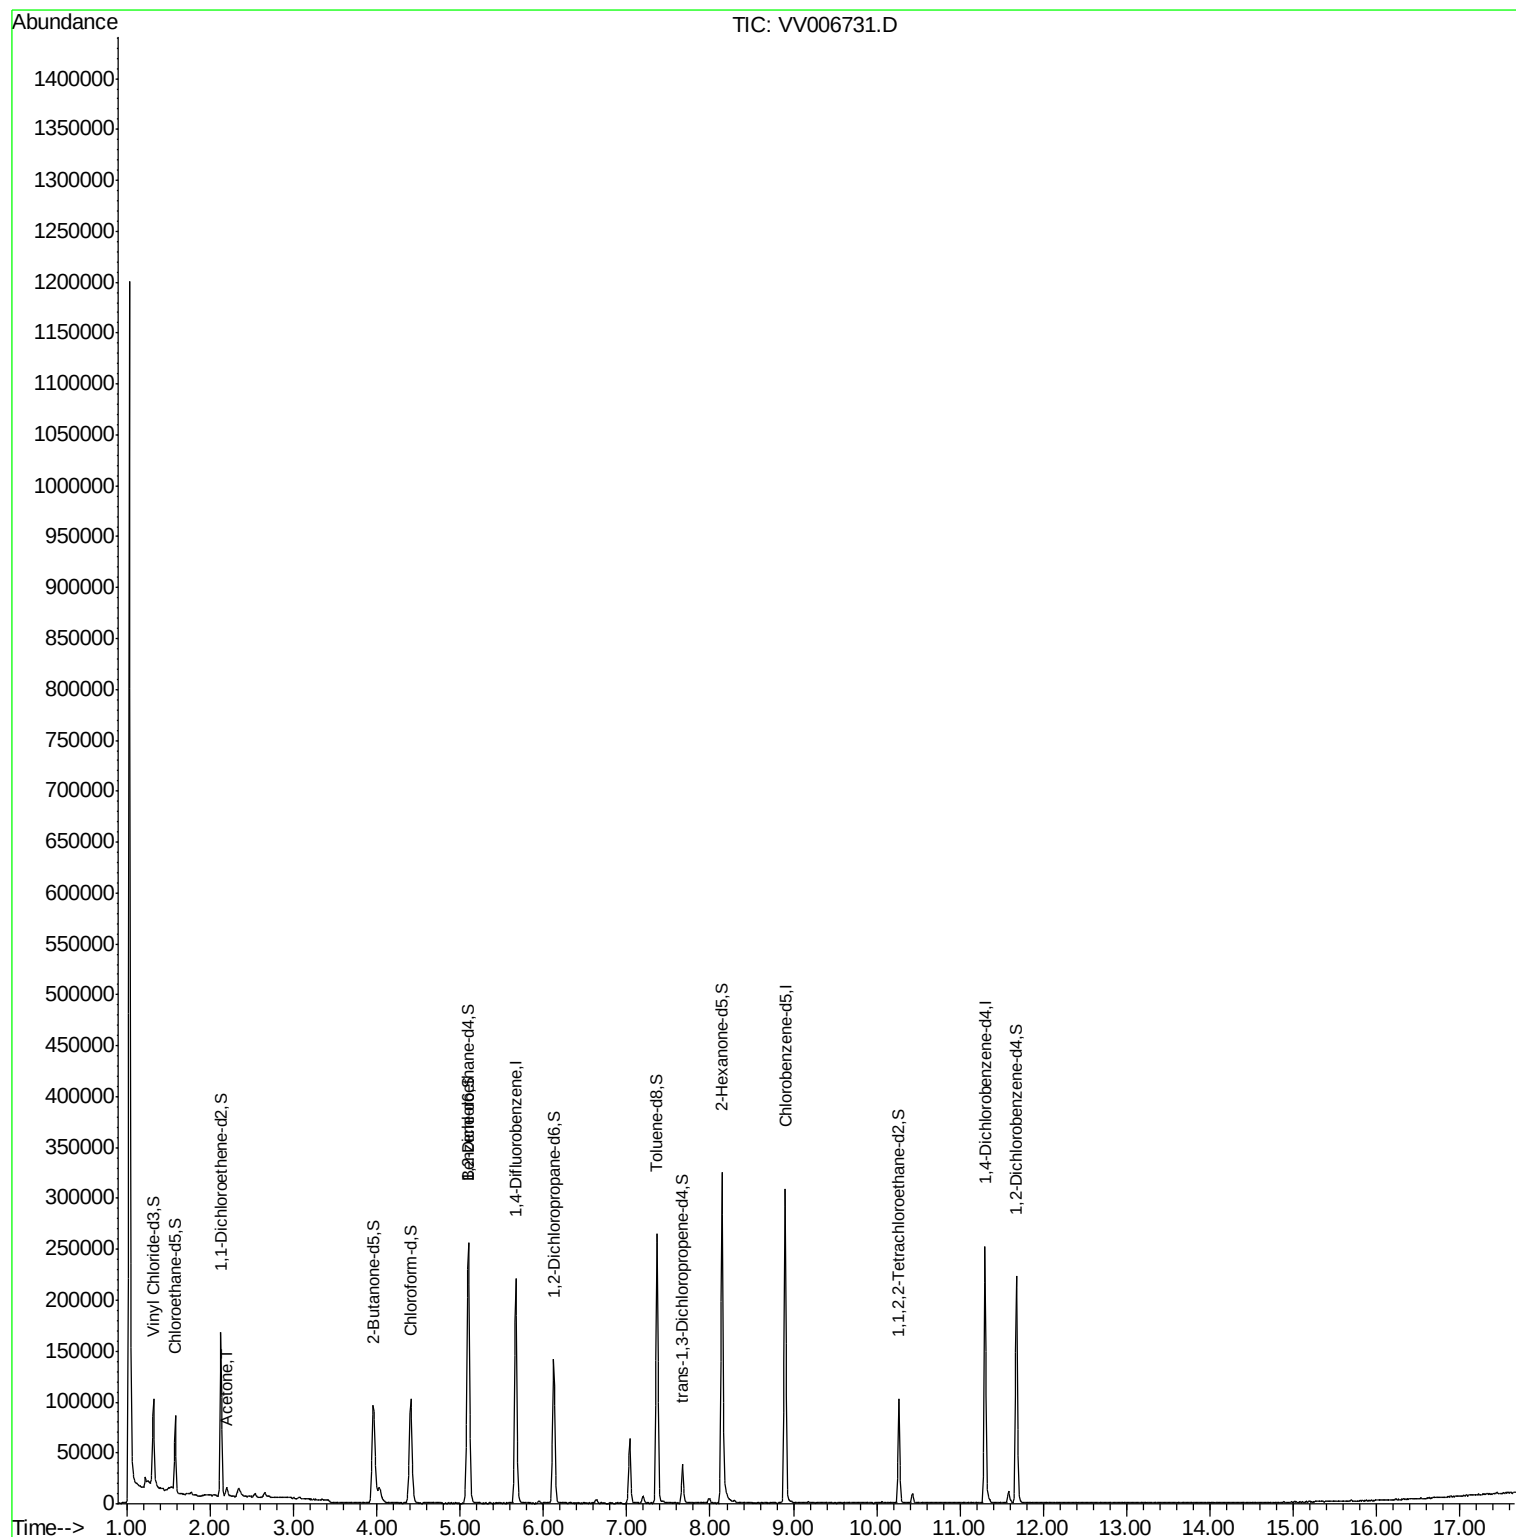

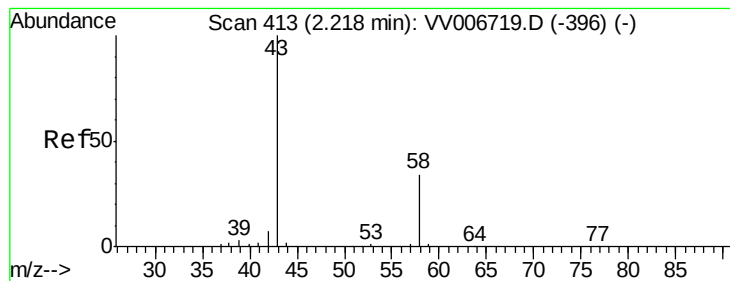

#13
 Acetone
 Concen: 3.999 ug/L
 RT: 2.20 min Scan# 407
 Delta R.T. -0.02 min
 Lab File: VV006731.D
 Acq: 27 Jul 2018 17:21

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC4

Tot Ion: 43 Resp: 7749
 Ion Ratio Lower Upper
 43 100
 58 30.4 0.0 71.4

