

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072718\
 Data File : VV006732.D
 Acq On : 27 Jul 2018 17:48
 Operator : SY/MD
 Sample : J4209-10
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC6

Quant Time: Jul 28 03:41:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 28 02:24:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	209808	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	195248	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	79023	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	67730	6.20	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	124.00%
7) Chloroethane-d5	1.58	69	50944	5.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.80%
11) 1,1-Dichloroethene-d2	2.13	63	90854	4.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.80%
20) 2-Butanone-d5	3.97	46	175807	51.53	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.06%
24) Chloroform-d	4.41	84	115329	5.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.60%
26) 1,2-Dichloroethane-d4	5.09	65	60082	6.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.20%
32) Benzene-d6	5.10	84	240479	5.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	119.80%
36) 1,2-Dichloropropane-d6	6.12	67	78883	5.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	116.40%
41) Toluene-d8	7.37	98	199720	5.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.80%
43) trans-1,3-Dichloropropene-	7.67	79	23873	5.39	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	107.80%
46) 2-Hexanone-d5	8.14	63	133060	47.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.00%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	57061	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	72263	6.13	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.60%#


Target Compounds					Ovalue
13) Acetone	2.21	43	9025	4.158 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072718\
Data File : VV006732.D
Acq On : 27 Jul 2018 17:48
Operator : SY/MD
Sample : J4209-10
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC6

Quant Time: Jul 28 03:41:28 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 28 02:24:46 2018
Response via : Initial Calibration

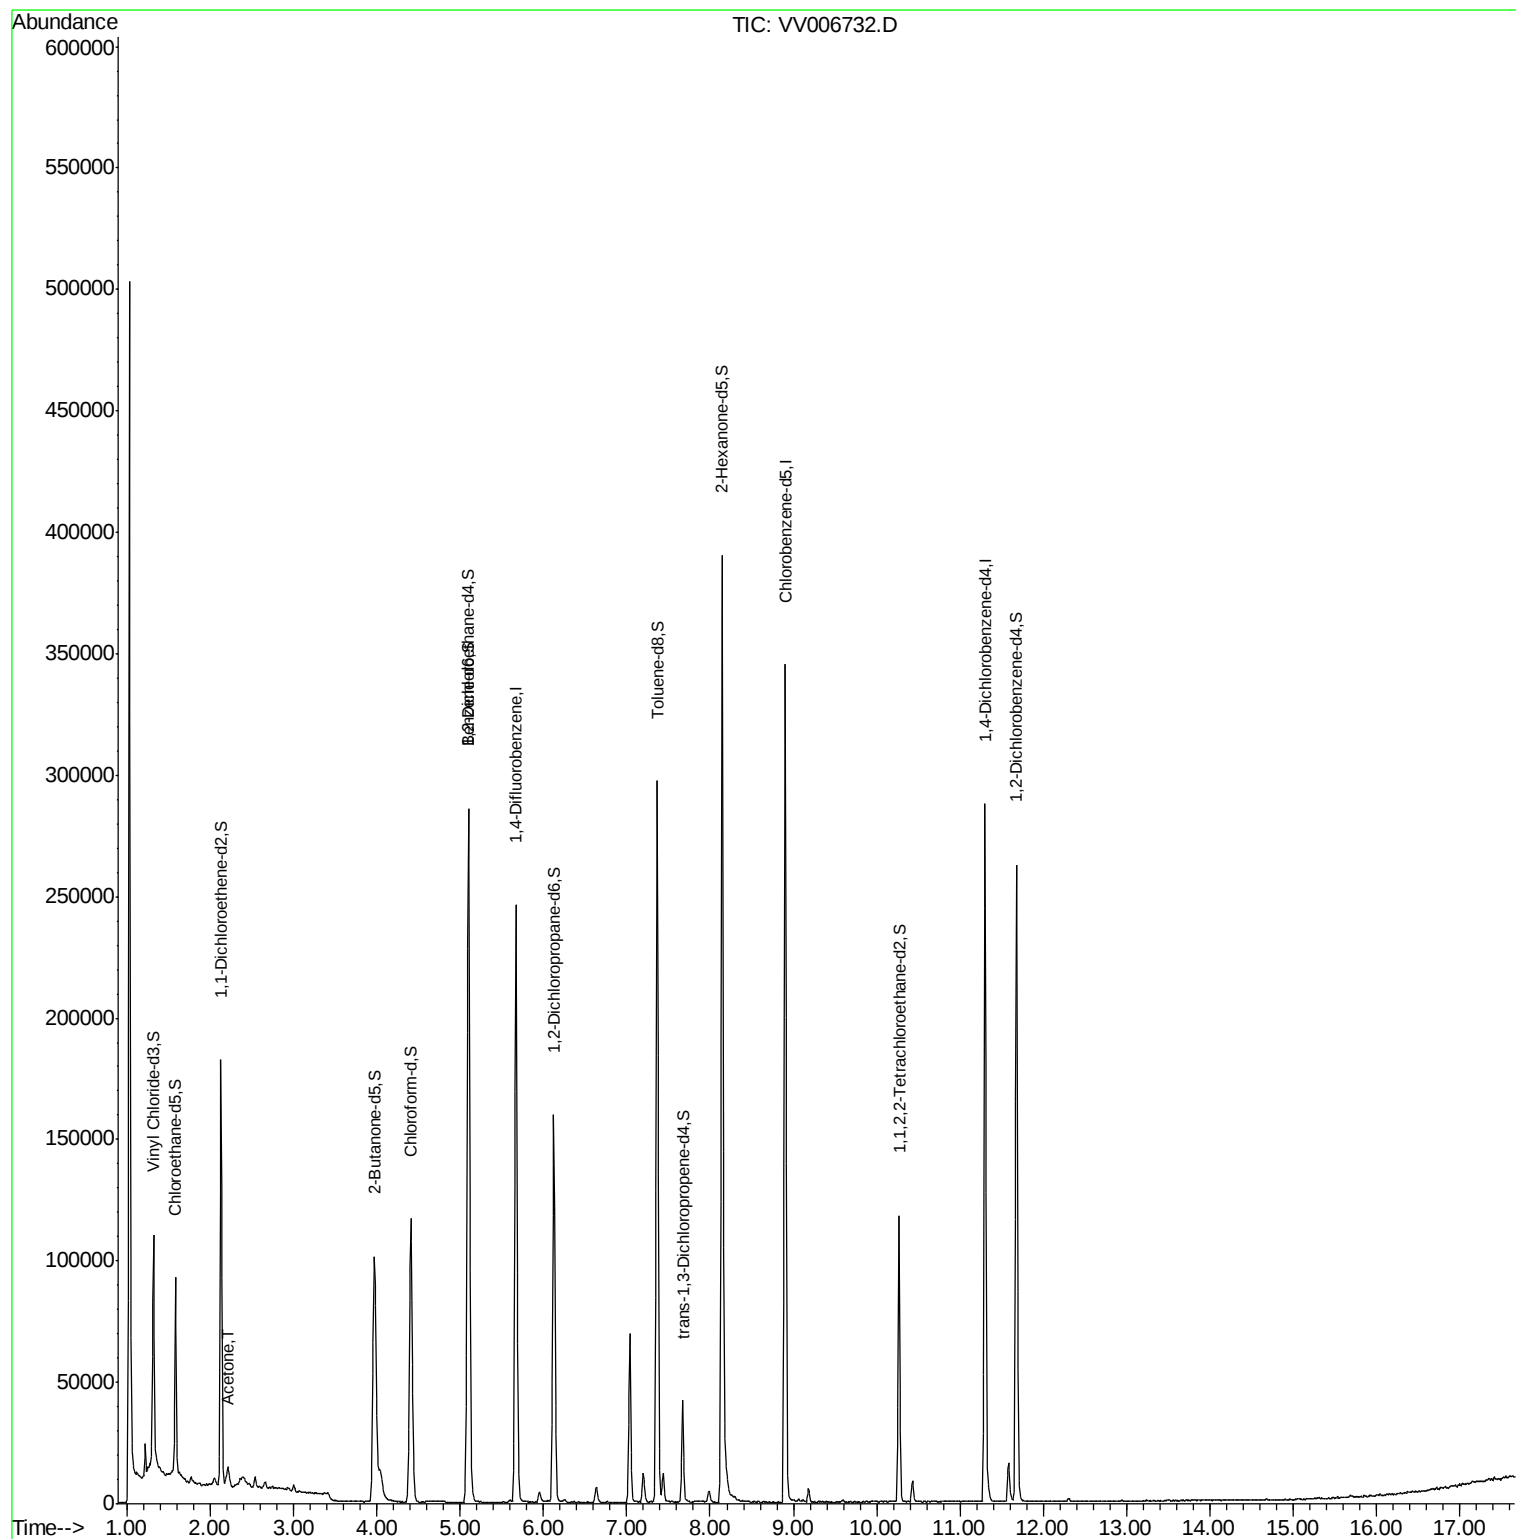

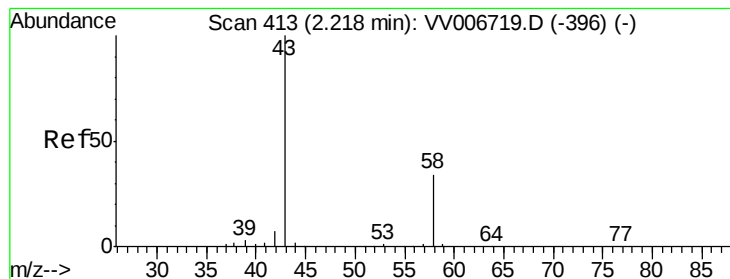

#13

Acetone

Concen: 4.158 ug/L

RT: 2.21 min Scan# 411

Delta R.T. -0.01 min

Lab File: VV006732.D

Acq: 27 Jul 2018 17:48

Instrument :
MSVOA_V
ClientSampleId :
C0AC6

Tot Ion: 43 Resp: 9025

Ion Ratio Lower Upper

43 100

58 37.6 0.0 71.4

