

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072718\
 Data File : VV006737.D
 Acq On : 27 Jul 2018 20:56
 Operator : SY/MD
 Sample : J4207-03
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JJ1G3

Quant Time: Jul 28 03:55:33 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 28 03:46:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	211636	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	198154	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	81748	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65333	5.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.60%
7) Chloroethane-d5	1.58	69	53514	6.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	123.80%
11) 1,1-Dichloroethene-d2	2.13	63	89106	4.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.40%
20) 2-Butanone-d5	3.95	46	187535	54.49	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.98%
24) Chloroform-d	4.41	84	118061	5.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.20%
26) 1,2-Dichloroethane-d4	5.09	65	61496	6.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	122.00%
32) Benzene-d6	5.10	84	240210	5.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	118.00%
36) 1,2-Dichloropropane-d6	6.12	67	79652	5.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.80%
41) Toluene-d8	7.36	98	197682	5.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.00%
43) trans-1,3-Dichloropropene-	7.67	79	24231	5.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	108.00%
46) 2-Hexanone-d5	8.14	63	145829	51.30	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.60%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	62249	5.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	74706	6.13	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.60%#


Target Compounds					Ovalue
13) Acetone	2.19	43	5286	2.41 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072718\
Data File : VV006737.D
Acq On : 27 Jul 2018 20:56
Operator : SY/MD
Sample : J4207-03
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JJ1G3

Quant Time: Jul 28 03:55:33 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 28 03:46:17 2018
Response via : Initial Calibration

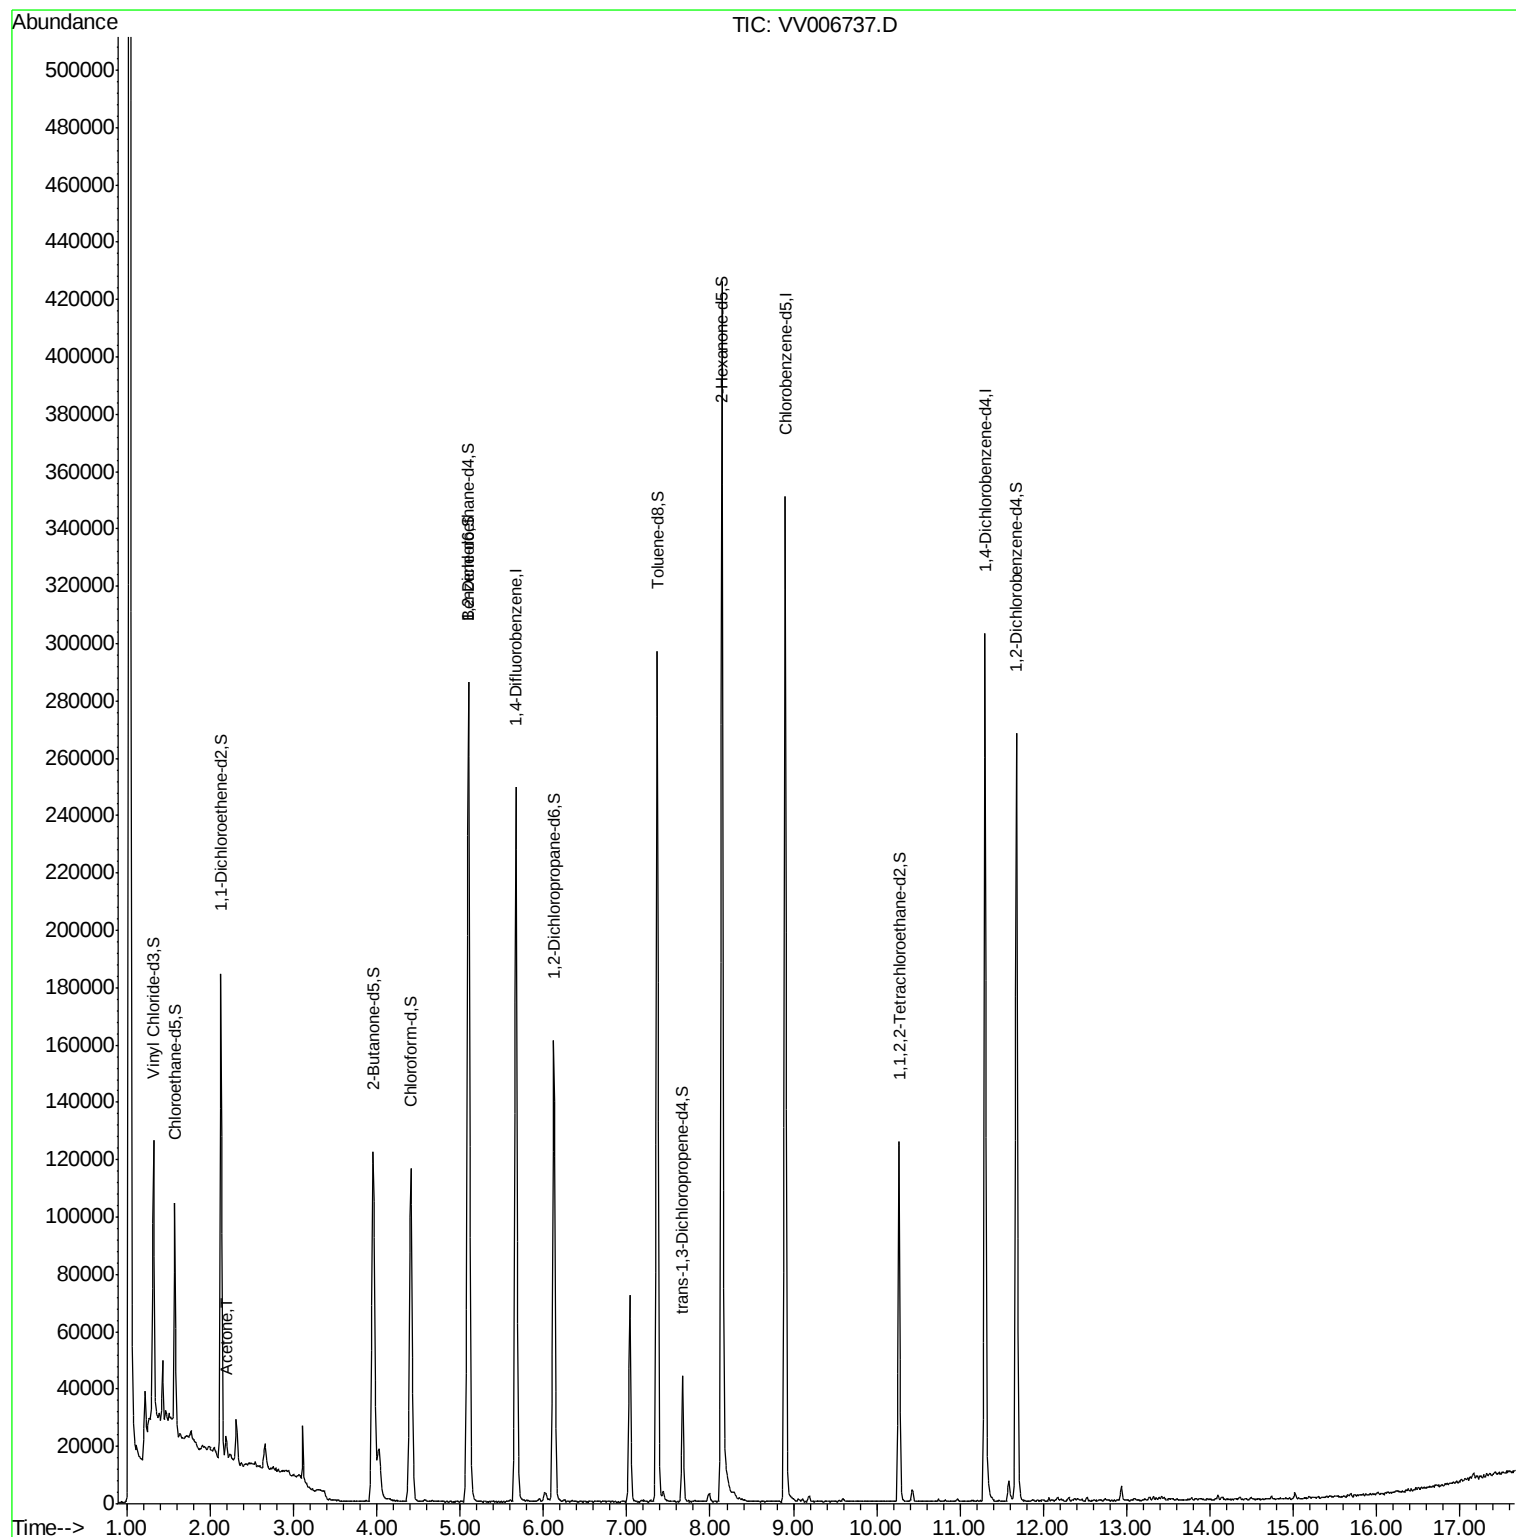

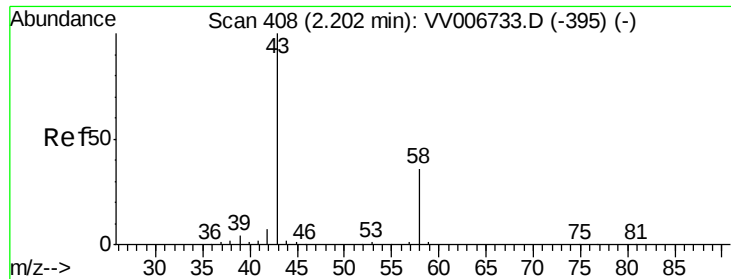

#13

Acetone

Concen: 2.41 ug/L

RT: 2.19 min Scan# 405

Delta R.T. -0.01 min

Lab File: VV006737.D

Acq: 27 Jul 2018 20:56

Instrument :
MSVOA_V
ClientSampleId :
JJ1G3

Tot Ion: 43 Resp: 5286

Ion Ratio Lower Upper

43 100

58 37.0 0.0 71.4

