

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072718\
 Data File : VV006745.D
 Acq On : 28 Jul 2018 00:31
 Operator : SY/MD
 Sample : J4207-11
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JJ1H1

Quant Time: Jul 28 04:33:03 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 28 03:46:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	220134	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	205700	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	83951	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65091	5.68	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.60%
7) Chloroethane-d5	1.57	69	53471	5.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.80%
11) 1,1-Dichloroethene-d2	2.13	63	88506	3.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.80%
20) 2-Butanone-d5	3.95	46	184725	51.60	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.20%
24) Chloroform-d	4.40	84	117495	5.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.40%
26) 1,2-Dichloroethane-d4	5.09	65	60852	5.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.20%
32) Benzene-d6	5.10	84	241001	5.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.00%
36) 1,2-Dichloropropane-d6	6.12	67	79358	5.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.20%
41) Toluene-d8	7.36	98	197061	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.60%
43) trans-1,3-Dichloropropene-	7.67	79	23291	5.00	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.00%
46) 2-Hexanone-d5	8.14	63	140535	47.62	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.24%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	60865	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	74360	5.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	5820	2.56 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072718\
Data File : VV006745.D
Acq On : 28 Jul 2018 00:31
Operator : SY/MD
Sample : J4207-11
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JJ1H1

Quant Time: Jul 28 04:33:03 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 28 03:46:17 2018
Response via : Initial Calibration

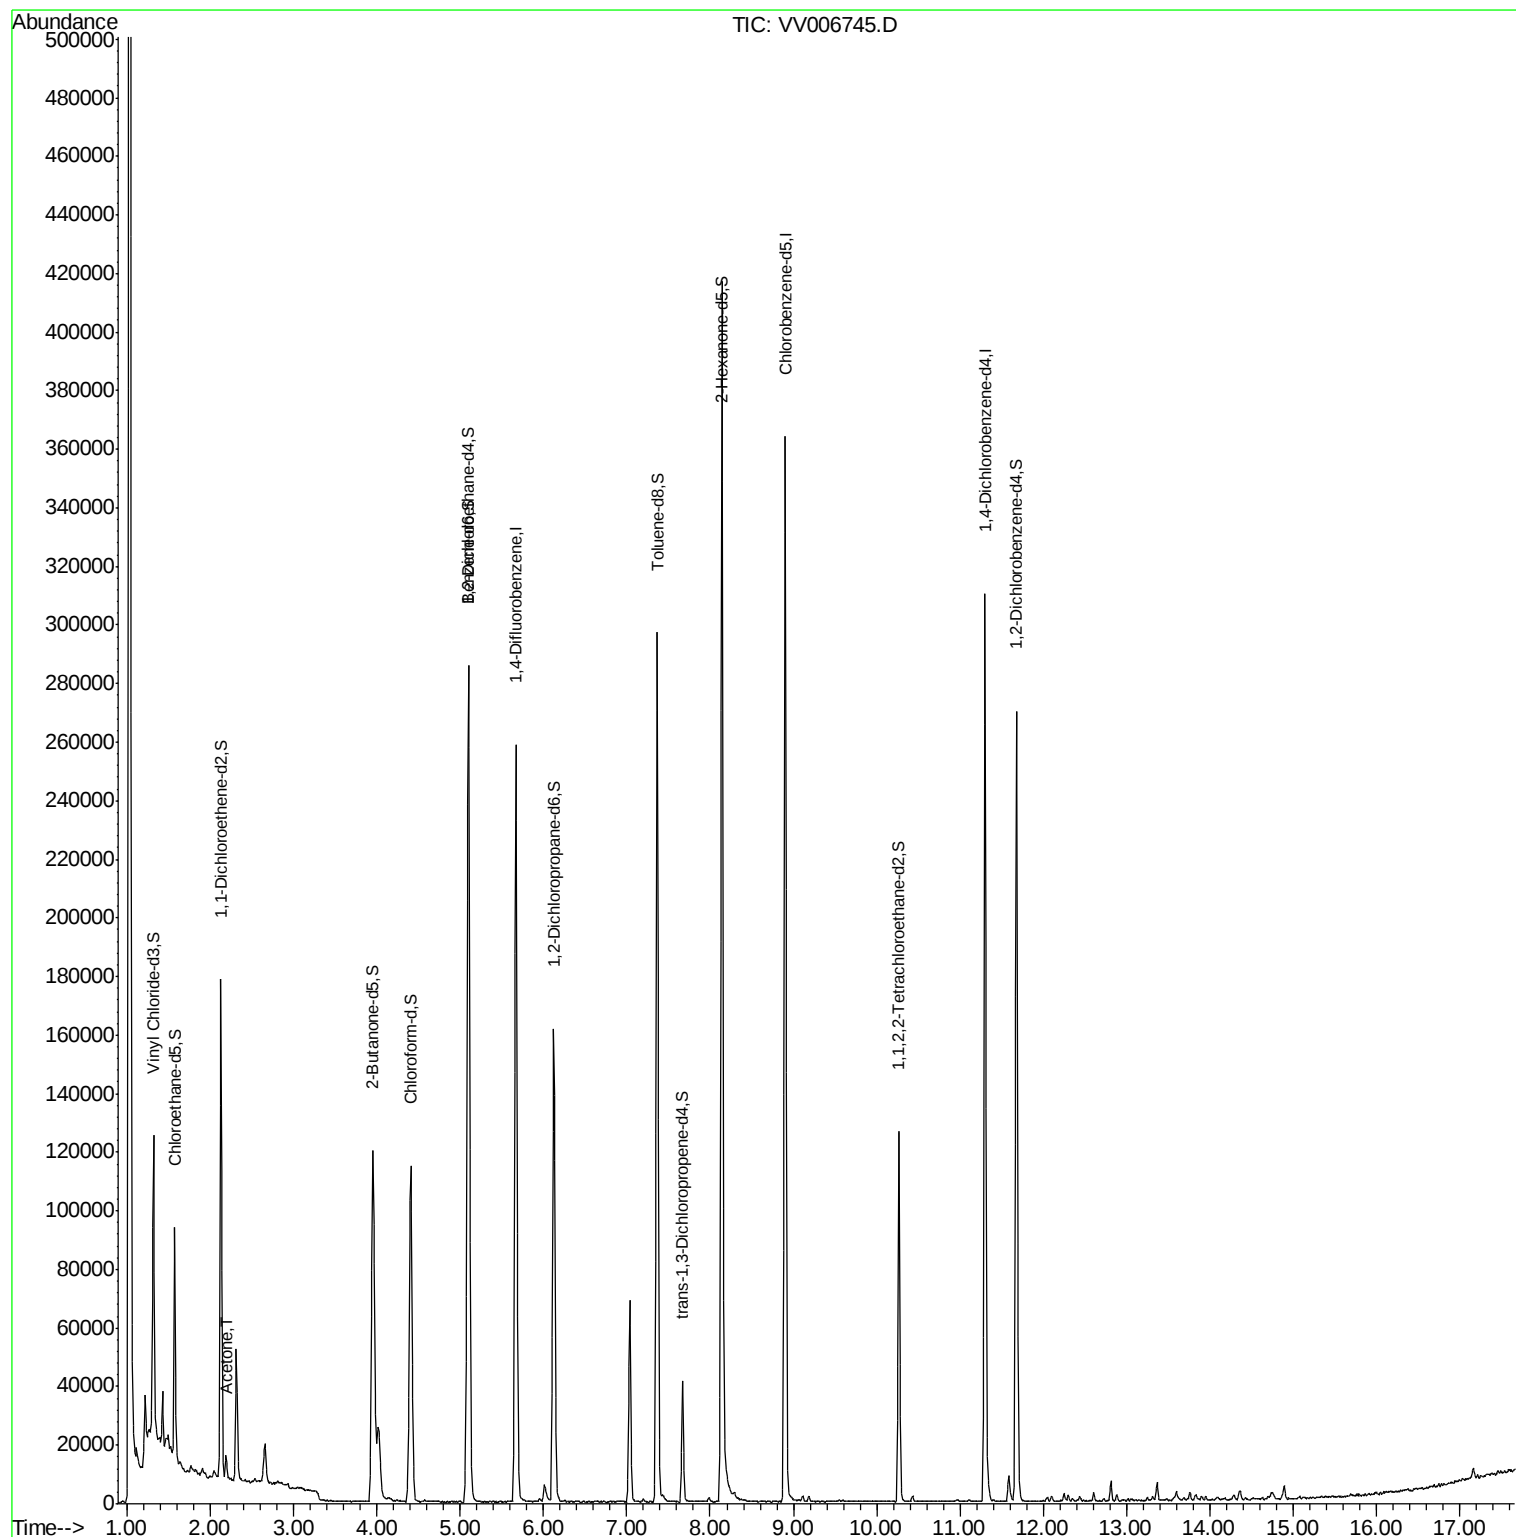

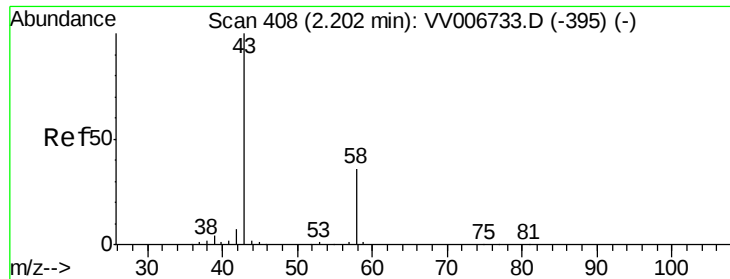

#13

Acetone

Concen: 2.56 ug/L

RT: 2.19 min Scan# 405

Delta R.T. -0.01 min

Lab File: VV006745.D

Acq: 28 Jul 2018 00:31

Instrument :
MSVOA_V
ClientSampleId :
JJ1H1

Tot Ion: 43 Resp: 5820

Ion Ratio Lower Upper

43 100

58 36.1 0.0 71.4

