

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072718\
 Data File : VV006748.D
 Acq On : 28 Jul 2018 01:51
 Operator : SY/MD
 Sample : J4207-14
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JJ1H4

Quant Time: Jul 28 04:42:30 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 28 03:46:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	226468	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	210514	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	84906	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65766	5.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.60%
7) Chloroethane-d5	1.58	69	52491	5.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.40%
11) 1,1-Dichloroethene-d2	2.13	63	89384	3.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.40%
20) 2-Butanone-d5	3.95	46	188427	51.16	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.32%
24) Chloroform-d	4.40	84	120688	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.20%
26) 1,2-Dichloroethane-d4	5.09	65	62020	5.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.00%
32) Benzene-d6	5.10	84	246197	5.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.80%
36) 1,2-Dichloropropane-d6	6.12	67	81994	5.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.20%
41) Toluene-d8	7.36	98	202513	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.00%
43) trans-1,3-Dichloropropene-	7.67	79	24263	5.09	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.80%
46) 2-Hexanone-d5	8.14	63	141774	46.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.88%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	60297	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	73851	5.84	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	6439	2.75 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072718\
Data File : VV006748.D
Acq On : 28 Jul 2018 01:51
Operator : SY/MD
Sample : J4207-14
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JJ1H4

Quant Time: Jul 28 04:42:30 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 28 03:46:17 2018
Response via : Initial Calibration

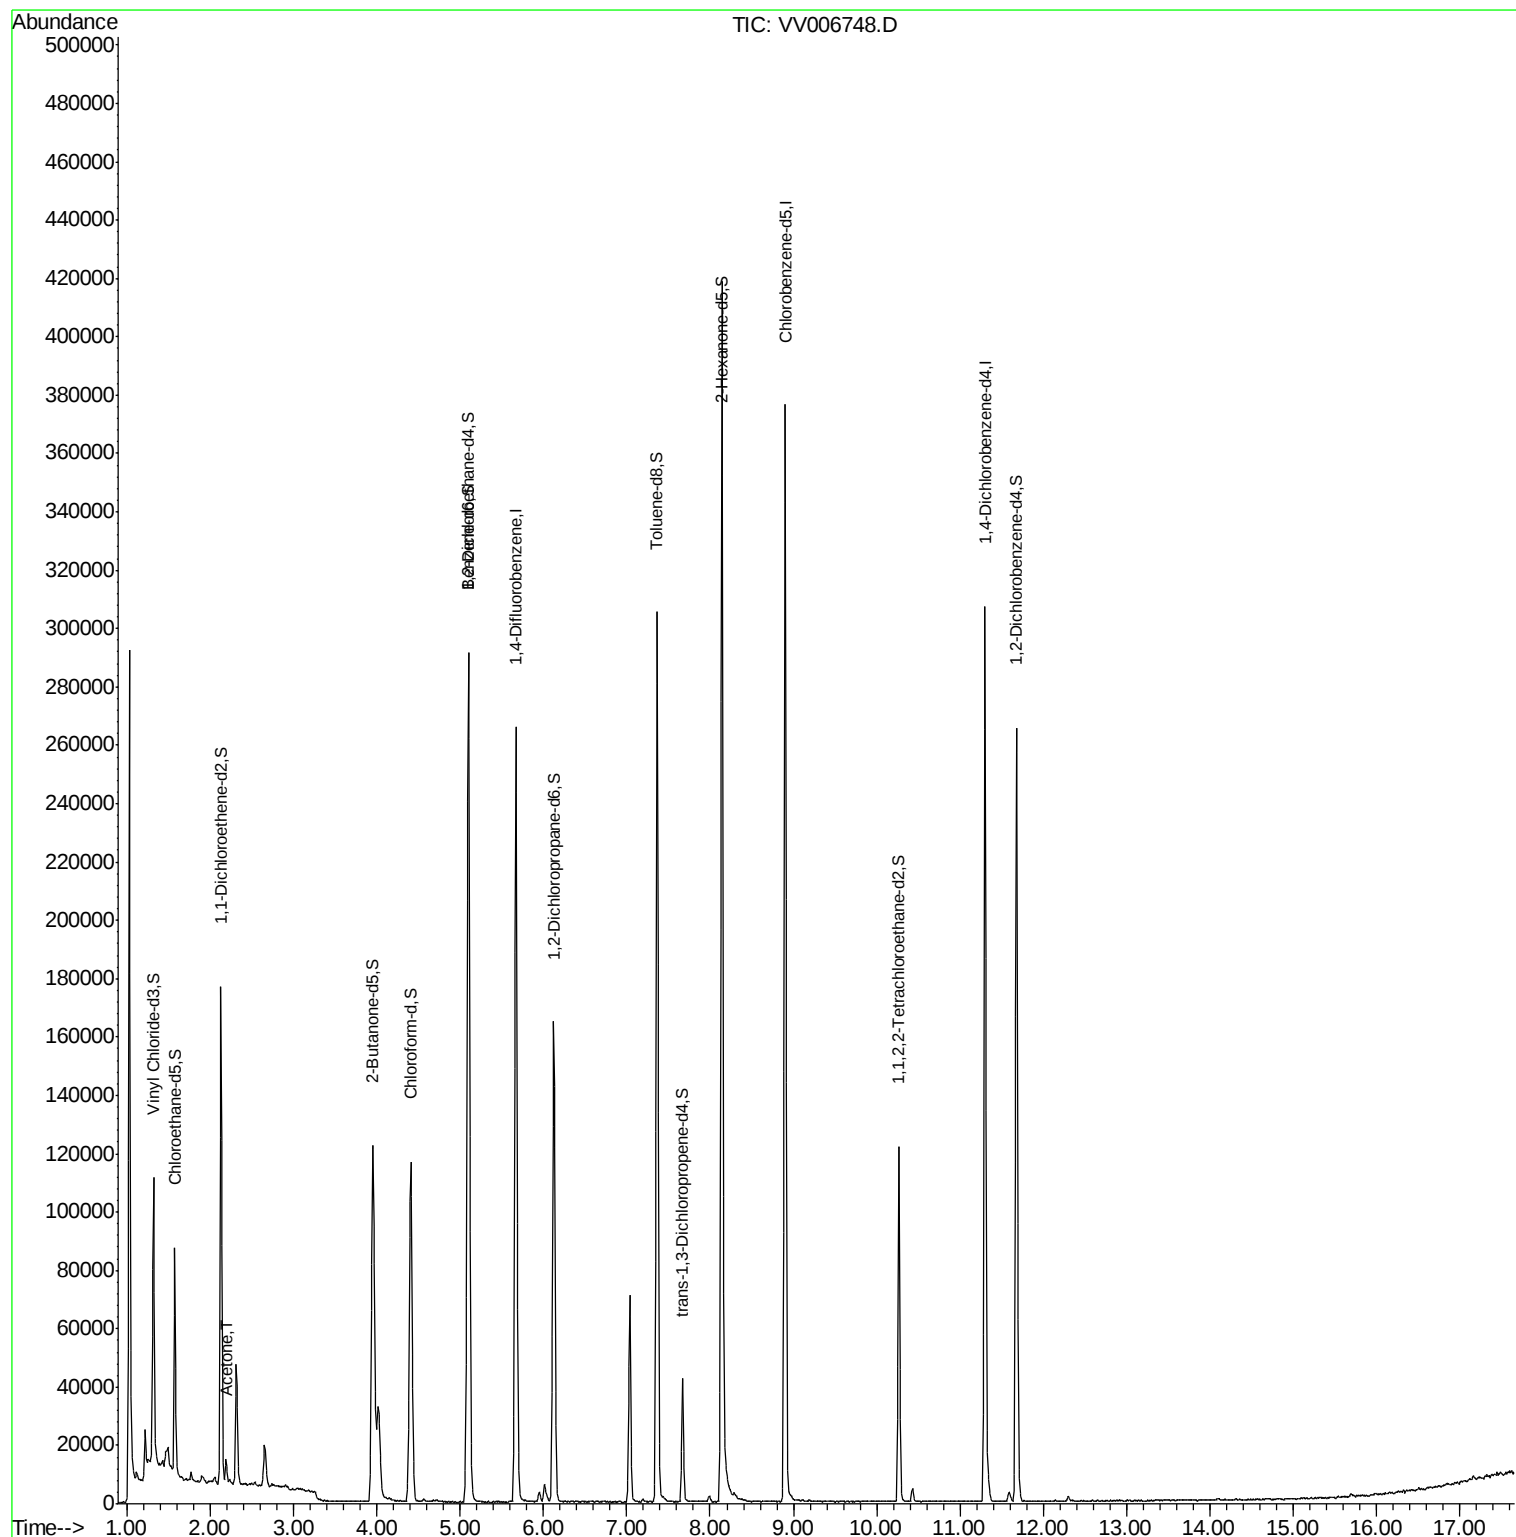

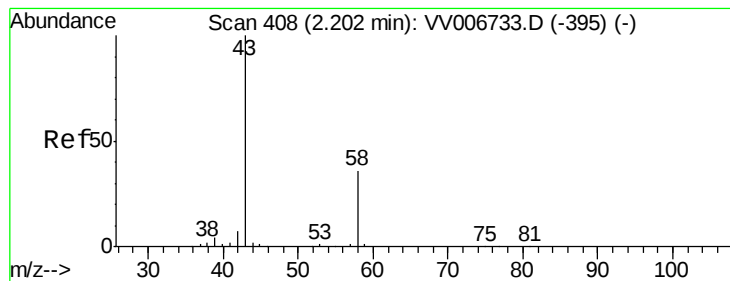

#13
 Acetone
 Concen: 2.75 ug/L
 RT: 2.19 min Scan# 404
 Delta R.T. -0.01 min
 Lab File: VV006748.D
 Acq: 28 Jul 2018 01:51

Instrument :
 MSVOA_V
 ClientSampleId :
 JJ1H4

Tot Ion: 43 Resp: 6439
 Ion Ratio Lower Upper
 43 100
 58 30.9 0.0 71.4

