

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072718\
 Data File : VV006750.D
 Acq On : 28 Jul 2018 02:45
 Operator : SY/MD
 Sample : J4207-16
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JJ1H8

Quant Time: Jul 28 04:47:14 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 28 03:46:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	225222	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	211193	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	94027	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	63913	5.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.00%
7) Chloroethane-d5	1.58	69	49912	5.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.40%
11) 1,1-Dichloroethene-d2	2.13	63	86691	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	3.96	46	179611	49.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.08%
24) Chloroform-d	4.41	84	116240	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.60%
26) 1,2-Dichloroethane-d4	5.09	65	60162	5.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.20%
32) Benzene-d6	5.10	84	236120	5.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.80%
36) 1,2-Dichloropropane-d6	6.12	67	79817	5.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.80%
41) Toluene-d8	7.36	98	196361	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
43) trans-1,3-Dichloropropene-	7.67	79	22654	4.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.60%
46) 2-Hexanone-d5	8.14	63	143021	47.20	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.40%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	59547	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	77034	5.50	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	5560	2.39 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072718\
Data File : VV006750.D
Acq On : 28 Jul 2018 02:45
Operator : SY/MD
Sample : J4207-16
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JJ1H8

Quant Time: Jul 28 04:47:14 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 28 03:46:17 2018
Response via : Initial Calibration

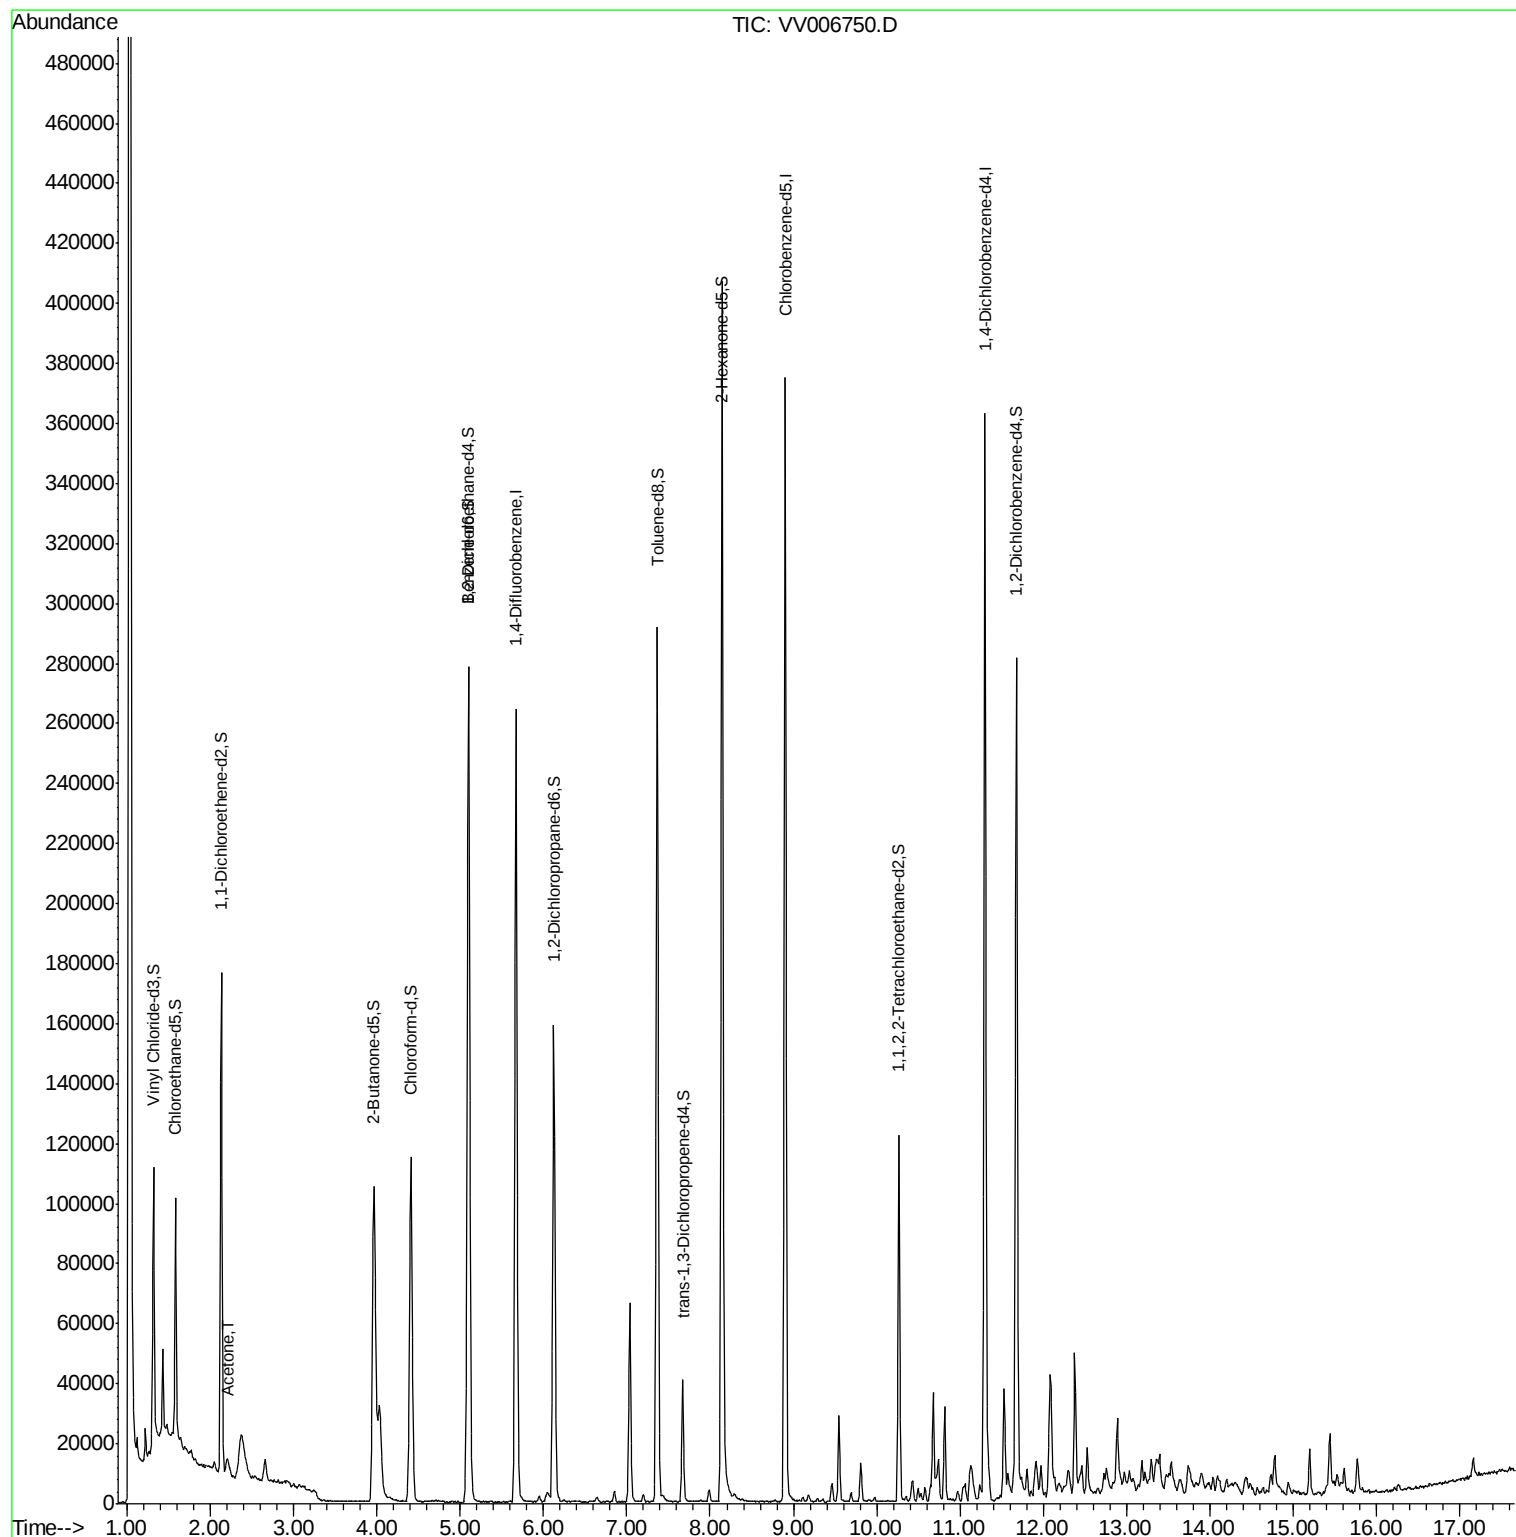

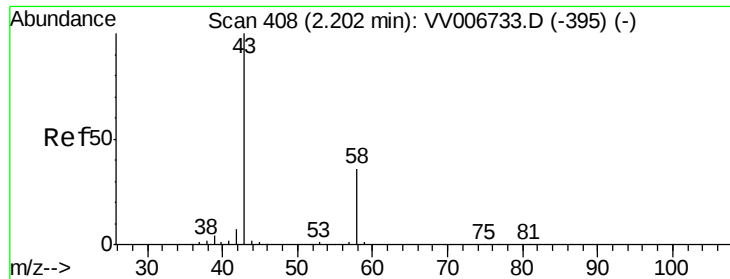

#13

Acetone

Concen: 2.39 ug/L

RT: 2.21 min Scan# 409

Delta R.T. 0.00 min

Lab File: VV006750.D

Acq: 28 Jul 2018 02:45

Instrument :
MSVOA_V
ClientSampleId :
JJ1H8

Tot Ion: 43 Resp: 5560

Ion Ratio Lower Upper

43 100

58 35.1 0.0 71.4

