

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072718\
 Data File : VV006752.D
 Acq On : 28 Jul 2018 03:38
 Operator : SY/MD
 Sample : J4207-19
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JJ1H6

Quant Time: Jul 28 05:04:25 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 28 03:46:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	222992	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	208663	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	84464	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	63489	5.47	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.40%
7) Chloroethane-d5	1.58	69	50855	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.60%
11) 1,1-Dichloroethene-d2	2.13	63	85188	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.80%
20) 2-Butanone-d5	3.96	46	181008	49.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.84%
24) Chloroform-d	4.41	84	114797	5.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.40%
26) 1,2-Dichloroethane-d4	5.09	65	59154	5.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.40%
32) Benzene-d6	5.10	84	234758	5.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.40%
36) 1,2-Dichloropropane-d6	6.12	67	76561	5.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.60%
41) Toluene-d8	7.37	98	191915	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.40%
43) trans-1,3-Dichloropropene-	7.67	79	22114	4.68	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.60%
46) 2-Hexanone-d5	8.14	63	137967	46.09	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.18%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	56775	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	70808	5.62	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	5711	2.48 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072718\
Data File : VV006752.D
Acq On : 28 Jul 2018 03:38
Operator : SY/MD
Sample : J4207-19
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JJ1H6

Quant Time: Jul 28 05:04:25 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 28 03:46:17 2018
Response via : Initial Calibration

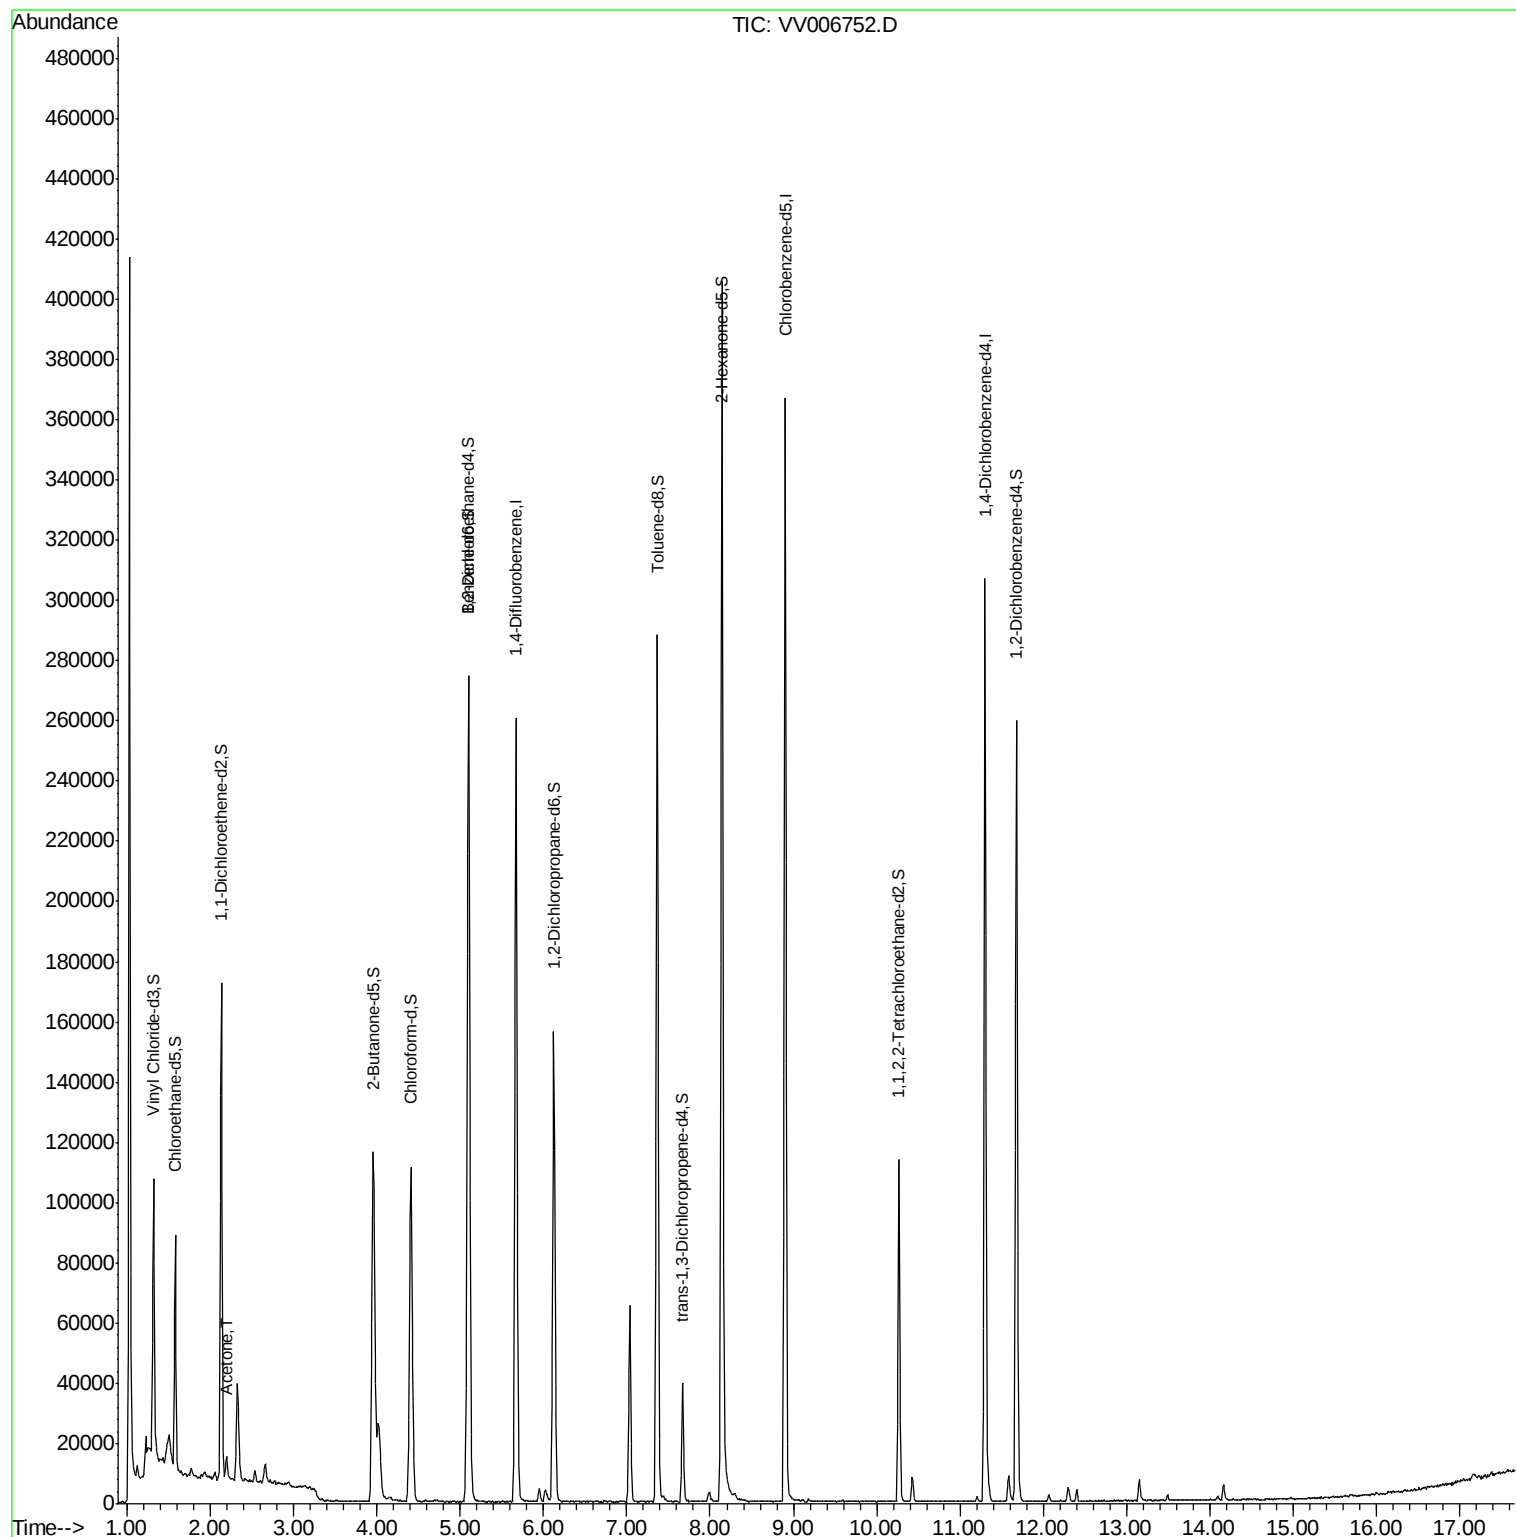

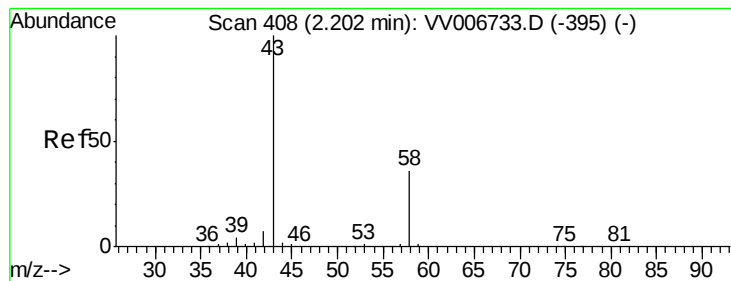

#13

Acetone

Concen: 2.48 ug/L

RT: 2.20 min Scan# 406

Delta R.T. -0.01 min

Lab File: VV006752.D

Acq: 28 Jul 2018 03:38

Instrument :
MSVOA_V
ClientSampleId :
JJ1H6

Tot Ion: 43 Resp: 5711

Ion Ratio Lower Upper

43 100

58 36.8 0.0 71.4

