

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027159.D
 Acq On : 02 Aug 2022 08:48
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK265

Quant Time: Aug 03 01:14:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 02 04:33:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	617683	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	597042	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	253243	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	229181	57.251	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 114.500%			
7) Chloroethane-d5	1.561	69	176737	58.999	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 118.000%			
11) 1,1-Dichloroethene-d2	2.101	63	290831	38.152	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 76.300%			
21) 2-Butanone-d5	3.880	46	278474	105.660	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 105.660%			
24) Chloroform-d	4.339	84	390077	48.207	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 96.420%			
26) 1,2-Dichloroethane-d4	5.024	65	234893	51.164	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.320%			
32) Benzene-d6	5.043	84	791719	50.113	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.220%			
36) 1,2-Dichloropropane-d6	6.066	67	251678	51.497	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 103.000%			
41) Toluene-d8	7.313	98	657390	46.156	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 92.320%			
43) trans-1,3-Dichloroprop...	7.619	79	103351	48.184	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 96.360%			
47) 2-Hexanone-d5	8.088	63	209253	110.905	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 110.900%			
56) 1,1,2,2-Tetrachloroeth...	10.214	84	366475	50.164	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 100.320%			
66) 1,2-Dichlorobenzene-d4	11.622	152	249805	56.128	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 112.260%			
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.246	75	28446	5.410	ug/L	# 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027159.D
Acq On : 02 Aug 2022 08:48
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK265

Quant Time: Aug 03 01:14:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 02 04:33:39 2022
Response via : Initial Calibration

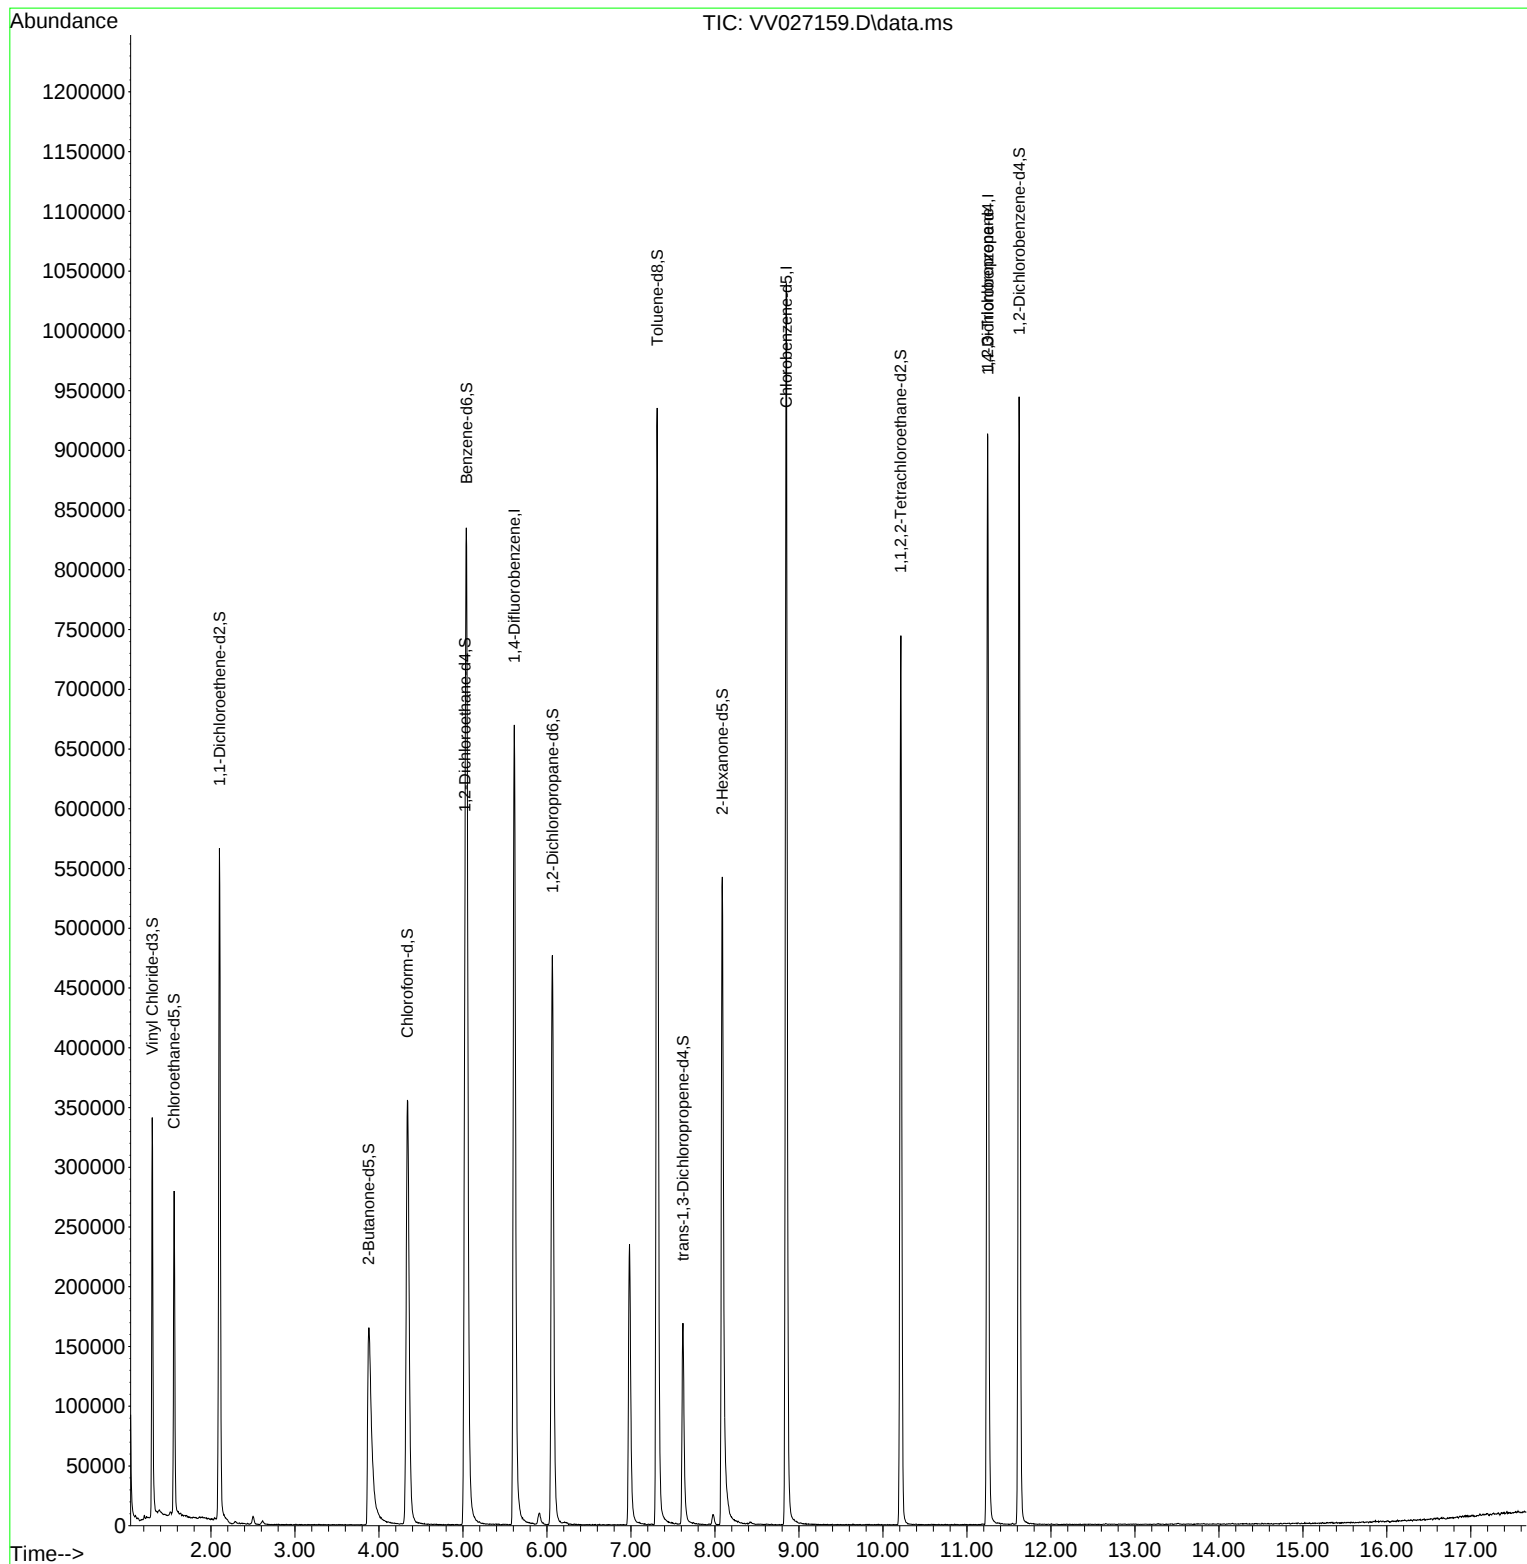

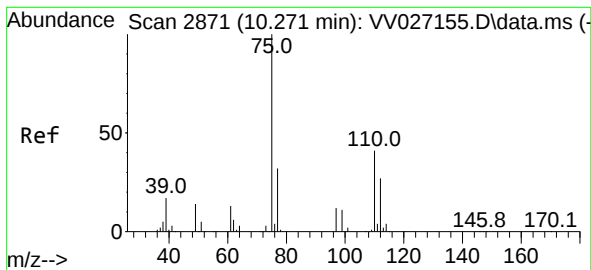

#61

1,2,3-Trichloropropane

Concen: 5.410 ug/L

RT: 11.246 min Scan# 31

Delta R.T. 0.974 min

Lab File: VV027159.D


Acq: 02 Aug 2022 08:48

Instrument :

MSVOA_V

ClientSampleId :

VIBLK265

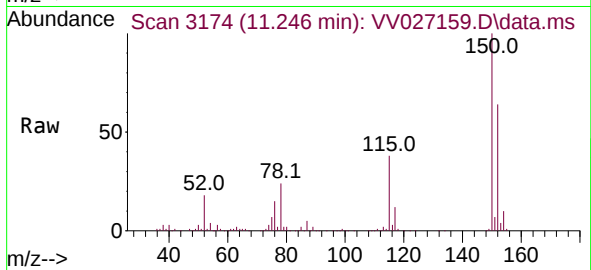

Tgt Ion: 75 Resp: 28446

Ion Ratio Lower Upper

75 100

77 31.7 25.8 38.8

110 2.5 32.8 49.2#

