

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027163.D
 Acq On : 02 Aug 2022 10:39
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK266

Quant Time: Aug 03 01:15:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 02 04:33:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	614325	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	601290	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	249644	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	225537	56.648	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	113.300%	
7) Chloroethane-d5	1.565	69	172086	57.760	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	115.520%	
11) 1,1-Dichloroethene-d2	2.105	63	288078	37.998	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	76.000%	
21) 2-Butanone-d5	3.880	46	284467	108.524	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	108.520%	
24) Chloroform-d	4.343	84	402331	49.993	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.980%	
26) 1,2-Dichloroethane-d4	5.027	65	239129	52.372	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	104.740%	
32) Benzene-d6	5.047	84	807417	50.746	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	101.500%	
36) 1,2-Dichloropropane-d6	6.066	67	256706	52.155	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	104.320%	
41) Toluene-d8	7.313	98	663057	46.225	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	92.440%	
43) trans-1,3-Dichloroprop...	7.619	79	111476	51.605	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	103.200%	
47) 2-Hexanone-d5	8.088	63	216767	114.075	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	114.080%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	378173	51.400	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	102.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	260638	59.406	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	118.820%	
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.982	75	6060	0.892	ug/L #	53
61) 1,2,3-Trichloropropane	11.246	75	27575	5.320	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027163.D
Acq On : 02 Aug 2022 10:39
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK266

Quant Time: Aug 03 01:15:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 02 04:33:39 2022
Response via : Initial Calibration

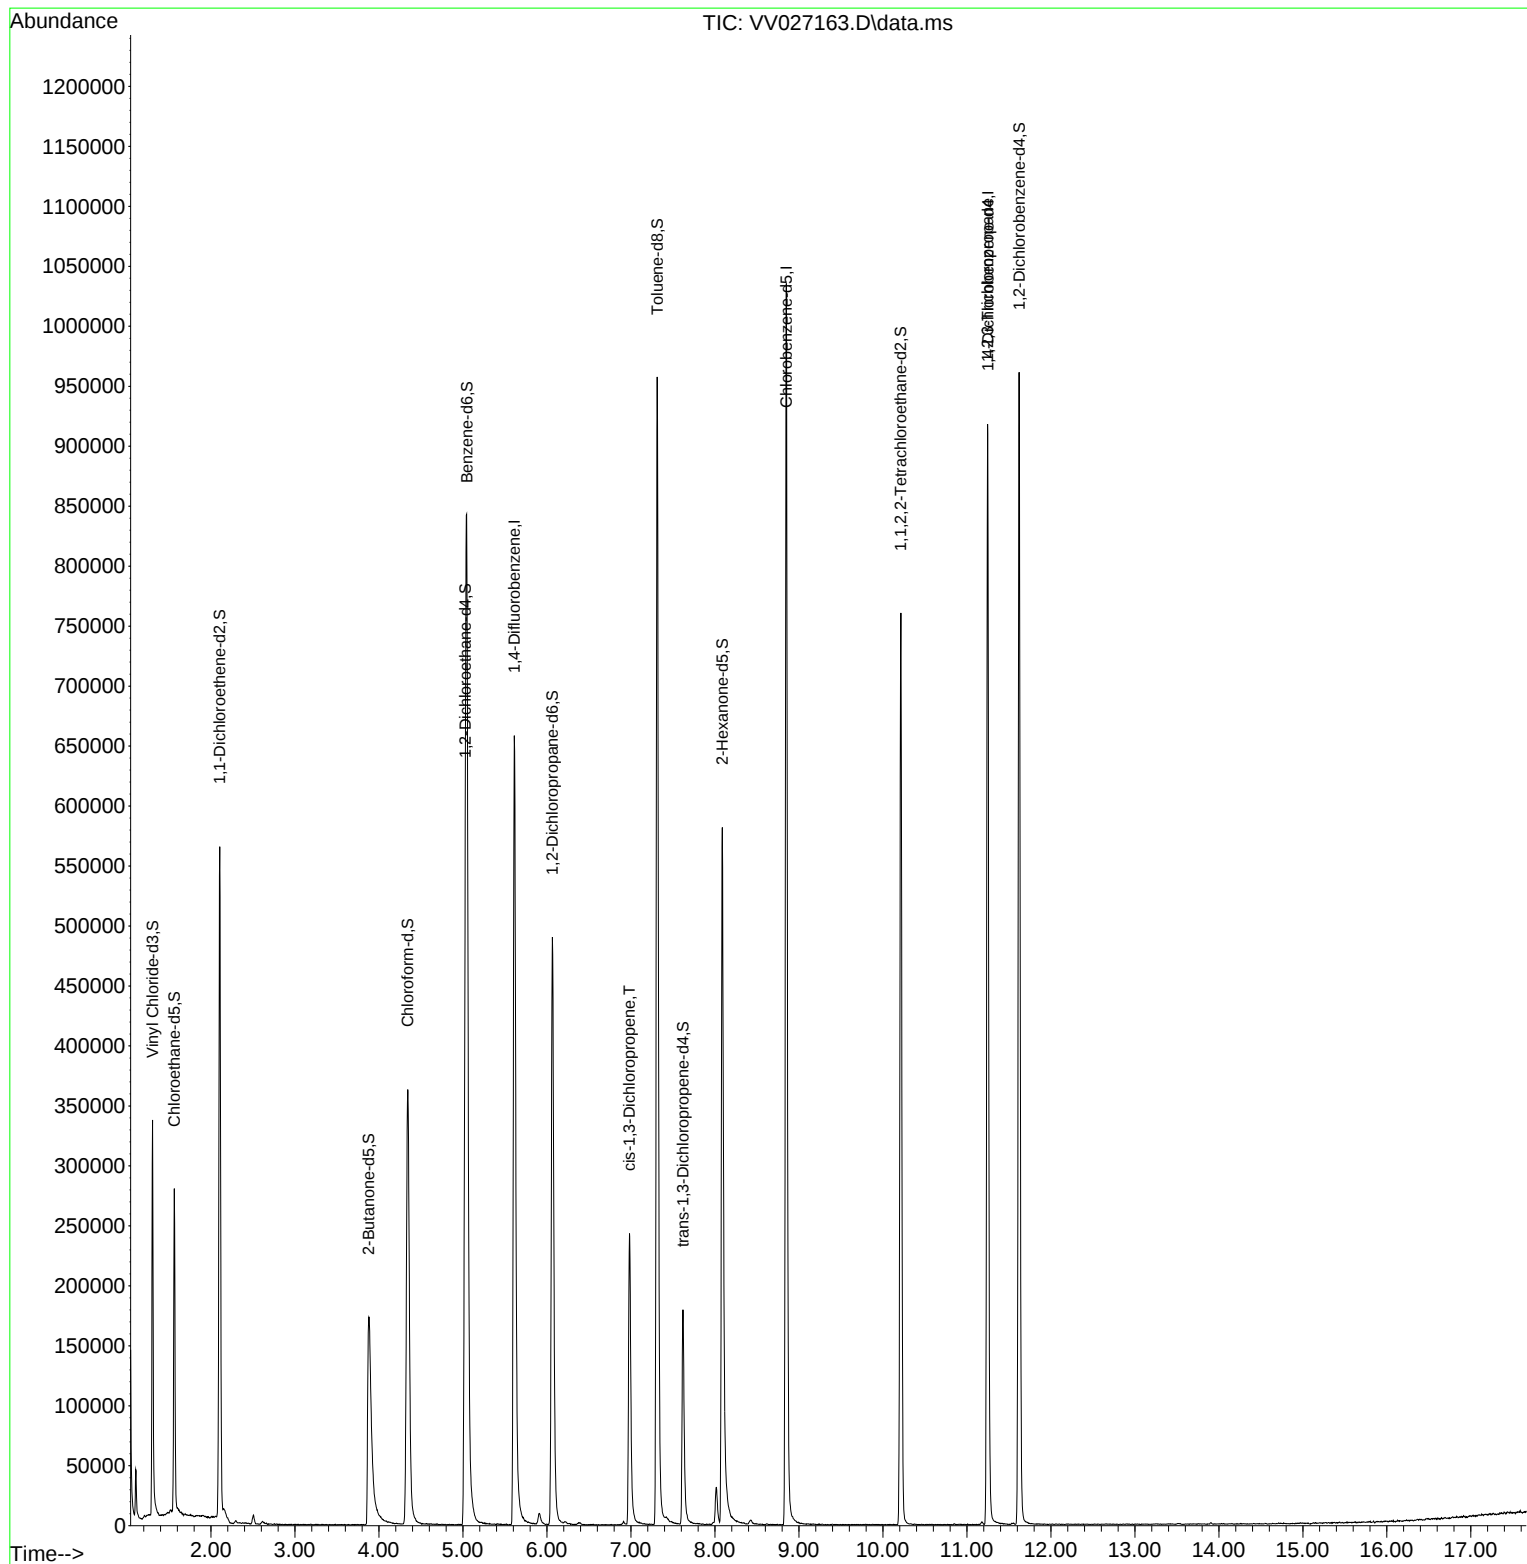

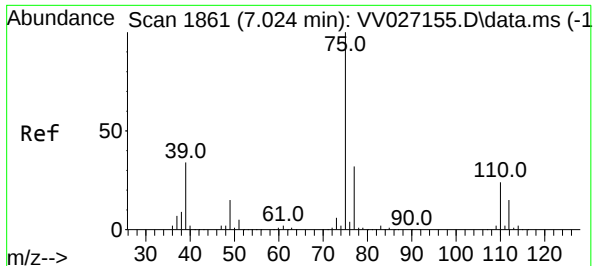

#39

cis-1,3-Dichloropropene

Concen: 0.892 ug/L

RT: 6.982 min Scan# 11

Delta R.T. -0.042 min

Lab File: VV027163.D

Acq: 02 Aug 2022 10:39

Instrument :

MSVOA_V

ClientSampleId :





VIBLK266

Tgt Ion: 75 Resp: 6060

Ion Ratio Lower Upper

75 100

77 57.9 22.3 41.5#

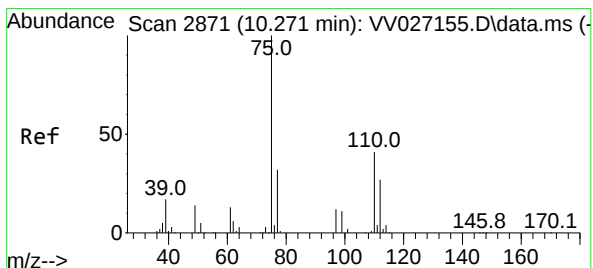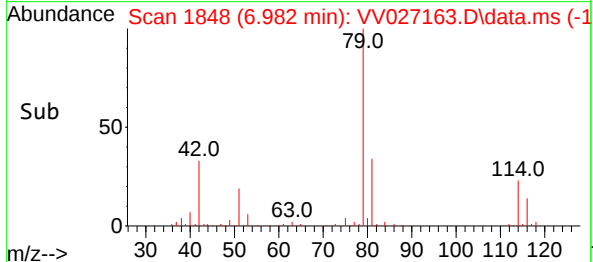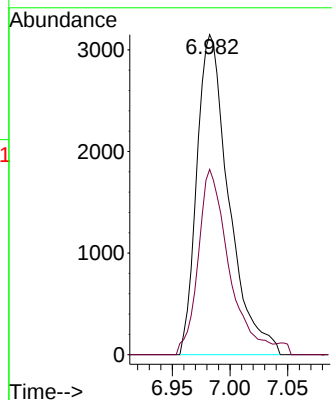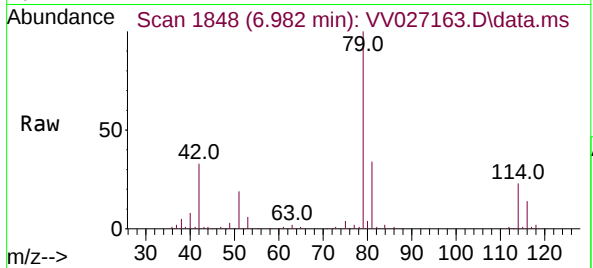

#61

1,2,3-Trichloropropane

Concen: 5.320 ug/L

RT: 11.246 min Scan# 3174

Delta R.T. 0.974 min

Lab File: VV027163.D

Acq: 02 Aug 2022 10:39

Tgt Ion: 75 Resp: 27575

Ion Ratio Lower Upper

75 100

77 33.2 25.8 38.8

110 2.6 32.8 49.2#

