

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW080122\
 Data File : VW027167.D
 Acq On : 02 Aug 2022 13:00
 Operator : SY/MD
 Sample : N3897-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Aug 03 01:16:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 02 04:33:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	576221	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	566283	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	236391	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	212934	57.019	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	114.040%
7) Chloroethane-d5	1.561	69	161683	57.857	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	115.720%
11) 1,1-Dichloroethene-d2	2.101	63	274140	38.551	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.100%
21) 2-Butanone-d5	3.876	46	287659	116.999	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	117.000%
24) Chloroform-d	4.342	84	387932	51.392	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.780%
26) 1,2-Dichloroethane-d4	5.027	65	226113	52.796	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.600%
32) Benzene-d6	5.043	84	773941	51.649	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.300%
36) 1,2-Dichloropropane-d6	6.066	67	248533	53.616	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.240%
41) Toluene-d8	7.313	98	635848	47.068	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.140%
43) trans-1,3-Dichloroprop...	7.619	79	101998	50.136	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.280%
47) 2-Hexanone-d5	8.088	63	212838	118.932	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	118.930%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	369509	53.327	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	106.660%
66) 1,2-Dichlorobenzene-d4	11.622	152	242161	58.289	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	116.580%
Target Compounds						
61) 1,2,3-Trichloropropane	11.246	75	26064	5.311	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027167.D
Acq On : 02 Aug 2022 13:00
Operator : SY/MD
Sample : N3897-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Aug 03 01:16:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 02 04:33:39 2022
Response via : Initial Calibration

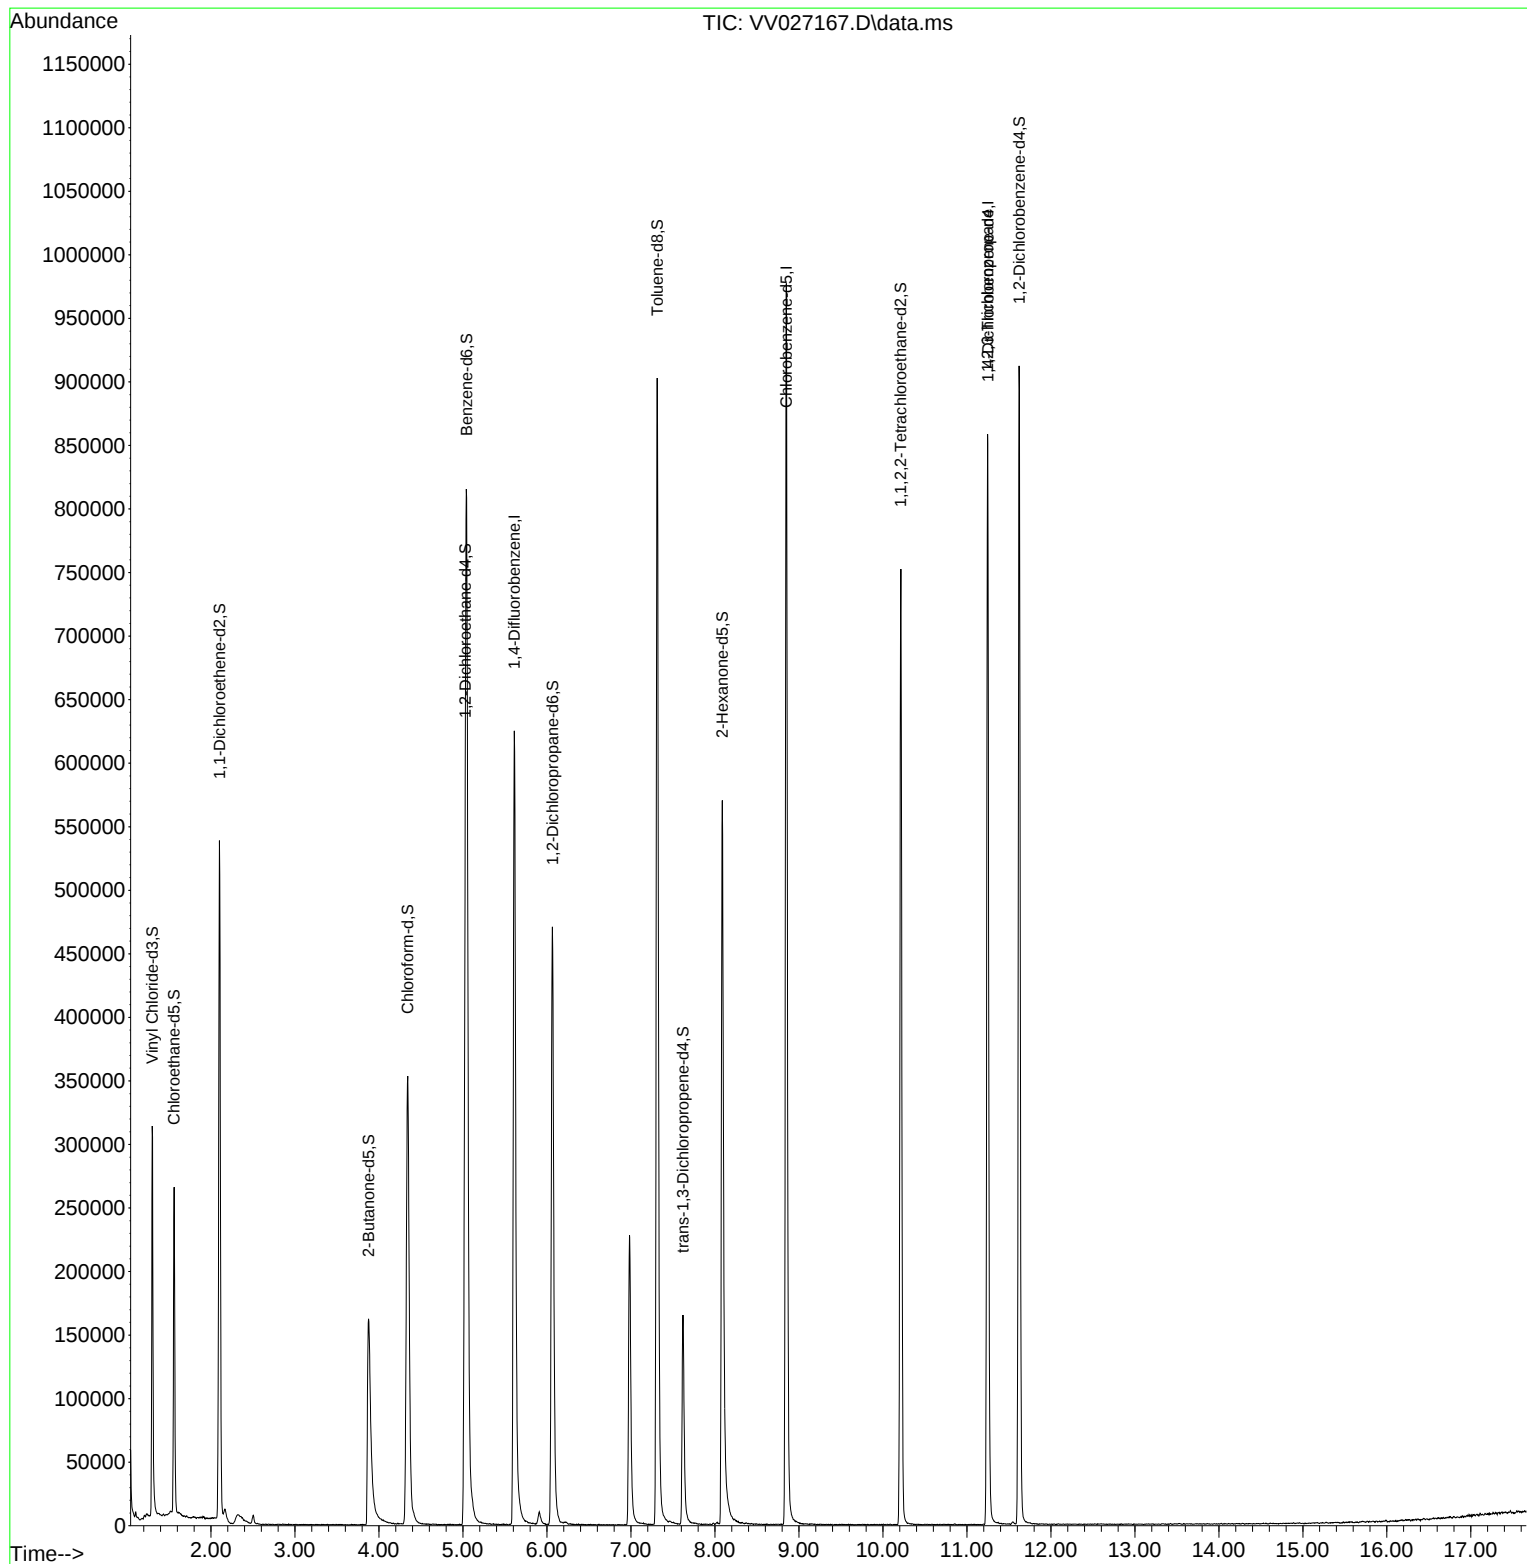

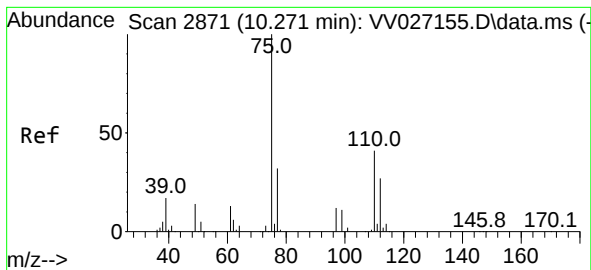

#61

1,2,3-Trichloropropane

Concen: 5.311 ug/L

RT: 11.246 min Scan# 31

Delta R.T. 0.974 min

Lab File: VV027167.D


Acq: 02 Aug 2022 13:00

Instrument :

MSVOA_V

ClientSampleId :

VHBLK001

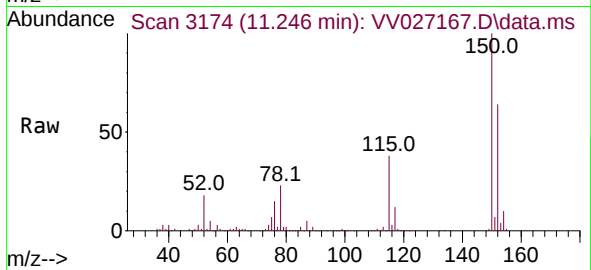

Tgt Ion: 75 Resp: 26064

Ion Ratio Lower Upper

75 100

77 32.0 25.8 38.8

110 2.5 32.8 49.2#

