

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027168.D
 Acq On : 02 Aug 2022 13:25
 Operator : SY/MD
 Sample : N3899-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Aug 03 01:16:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 02 04:33:39 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	599816	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	589010	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	242780	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	219692	56.515	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	113.020%	
7) Chloroethane-d5	1.564	69	163269	56.127	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	112.260%	
11) 1,1-Dichloroethene-d2	2.105	63	278559	37.631	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	75.260%	
21) 2-Butanone-d5	3.876	46	281347	109.930	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	109.930%	
24) Chloroform-d	4.342	84	398395	50.702	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	101.400%	
26) 1,2-Dichloroethane-d4	5.027	65	239039	53.618	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	107.240%	
32) Benzene-d6	5.047	84	787956	50.555	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	101.120%	
36) 1,2-Dichloropropane-d6	6.066	67	256390	53.177	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	106.360%	
41) Toluene-d8	7.313	98	646185	45.988	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	91.980%	
43) trans-1,3-Dichloroprop...	7.619	79	104305	49.292	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	98.580%	
47) 2-Hexanone-d5	8.088	63	223748	120.204	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	120.200%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	379227	52.618	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	105.240%	
66) 1,2-Dichlorobenzene-d4	11.622	152	248760	58.302	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	116.600%	
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.246	75	27456	5.447	ug/L	# 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027168.D
Acq On : 02 Aug 2022 13:25
Operator : SY/MD
Sample : N3899-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Aug 03 01:16:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 02 04:33:39 2022
Response via : Initial Calibration

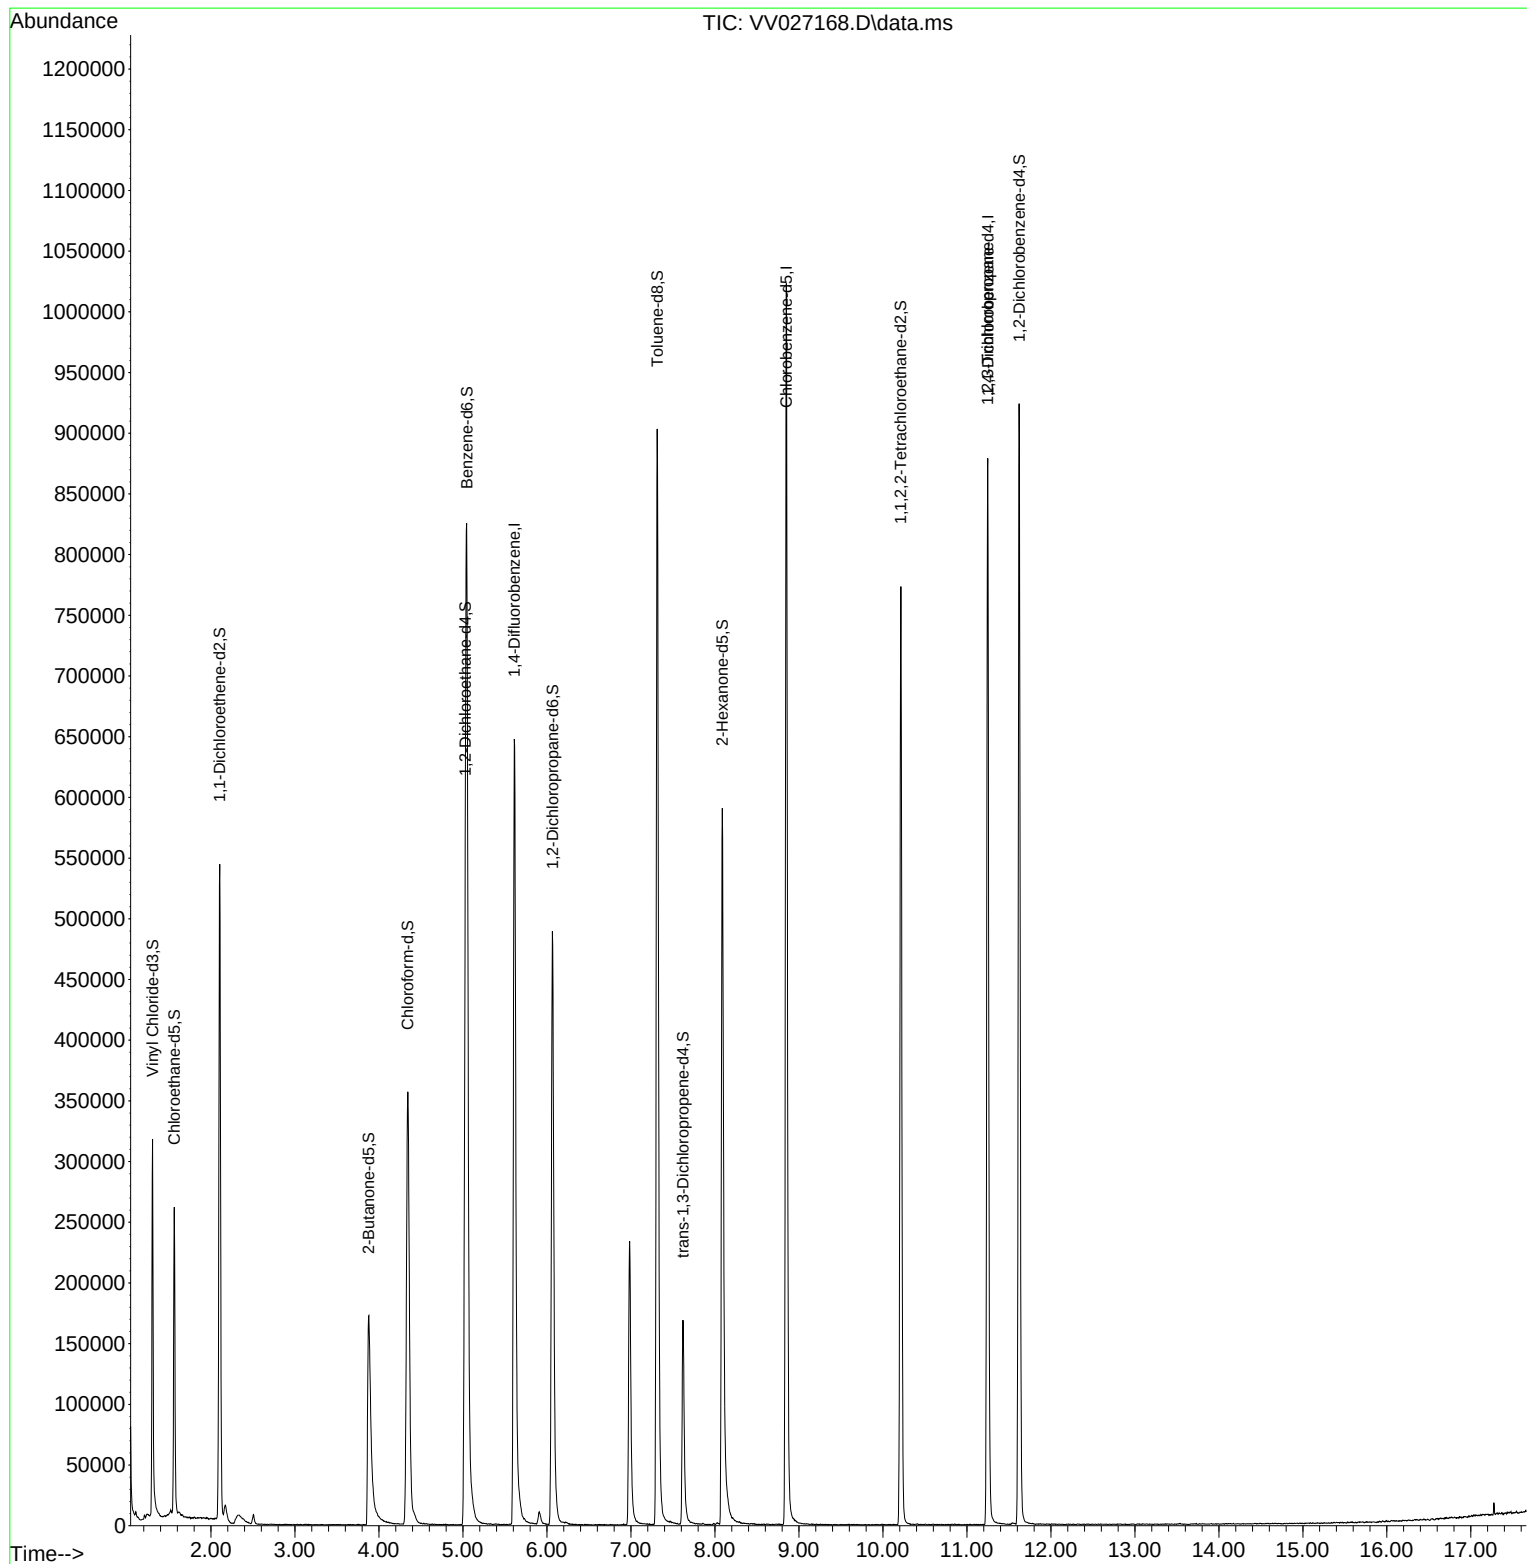

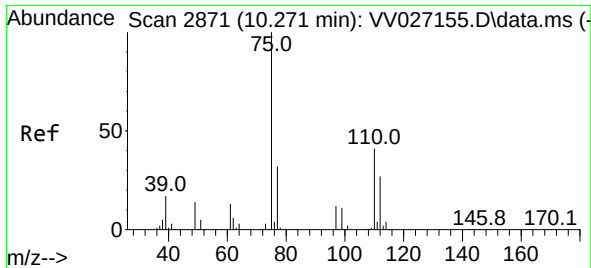

#61

1,2,3-Trichloropropane

Concen: 5.447 ug/L

RT: 11.246 min Scan# 31

Delta R.T. 0.974 min

Lab File: VV027168.D


Acq: 02 Aug 2022 13:25

Instrument :

MSVOA_V

ClientSampleId :

VHBLK001

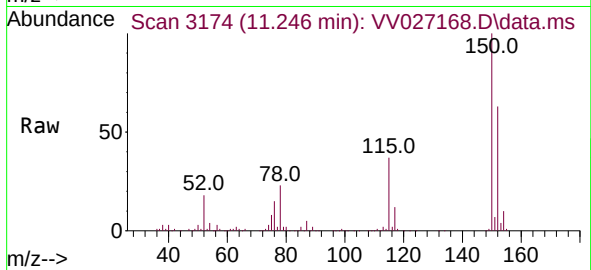

Tgt Ion: 75 Resp: 27456

Ion Ratio Lower Upper

75 100

77 31.4 25.8 38.8

110 2.4 32.8 49.2#

