

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027169.D
 Acq On : 02 Aug 2022 13:49
 Operator : SY/MD
 Sample : N3880-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Aug 03 01:16:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 02 04:33:39 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	589465	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	579158	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	239534	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	219899	57.561	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	115.120%	
7) Chloroethane-d5	1.561	69	163982	57.362	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	114.720%	
11) 1,1-Dichloroethene-d2	2.105	63	277466	38.142	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	76.280%	
21) 2-Butanone-d5	3.880	46	286807	114.031	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	114.030%	
24) Chloroform-d	4.343	84	395712	51.245	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.480%	
26) 1,2-Dichloroethane-d4	5.027	65	235282	53.702	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	107.400%	
32) Benzene-d6	5.047	84	785590	51.261	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.520%	
36) 1,2-Dichloropropane-d6	6.066	67	252190	53.196	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	106.400%	
41) Toluene-d8	7.314	98	636783	46.090	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	92.180%	
43) trans-1,3-Dichloroprop...	7.619	79	102860	49.436	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	98.880%	
47) 2-Hexanone-d5	8.088	63	214802	117.361	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	117.360%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	372192	52.520	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	105.040%	
66) 1,2-Dichlorobenzene-d4	11.622	152	246904	58.651	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	117.300%	
Target Compounds						
61) 1,2,3-Trichloropropane	11.246	75	27261	5.482	ug/L	Qvalue # 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027169.D
Acq On : 02 Aug 2022 13:49
Operator : SY/MD
Sample : N3880-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Aug 03 01:16:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 02 04:33:39 2022
Response via : Initial Calibration

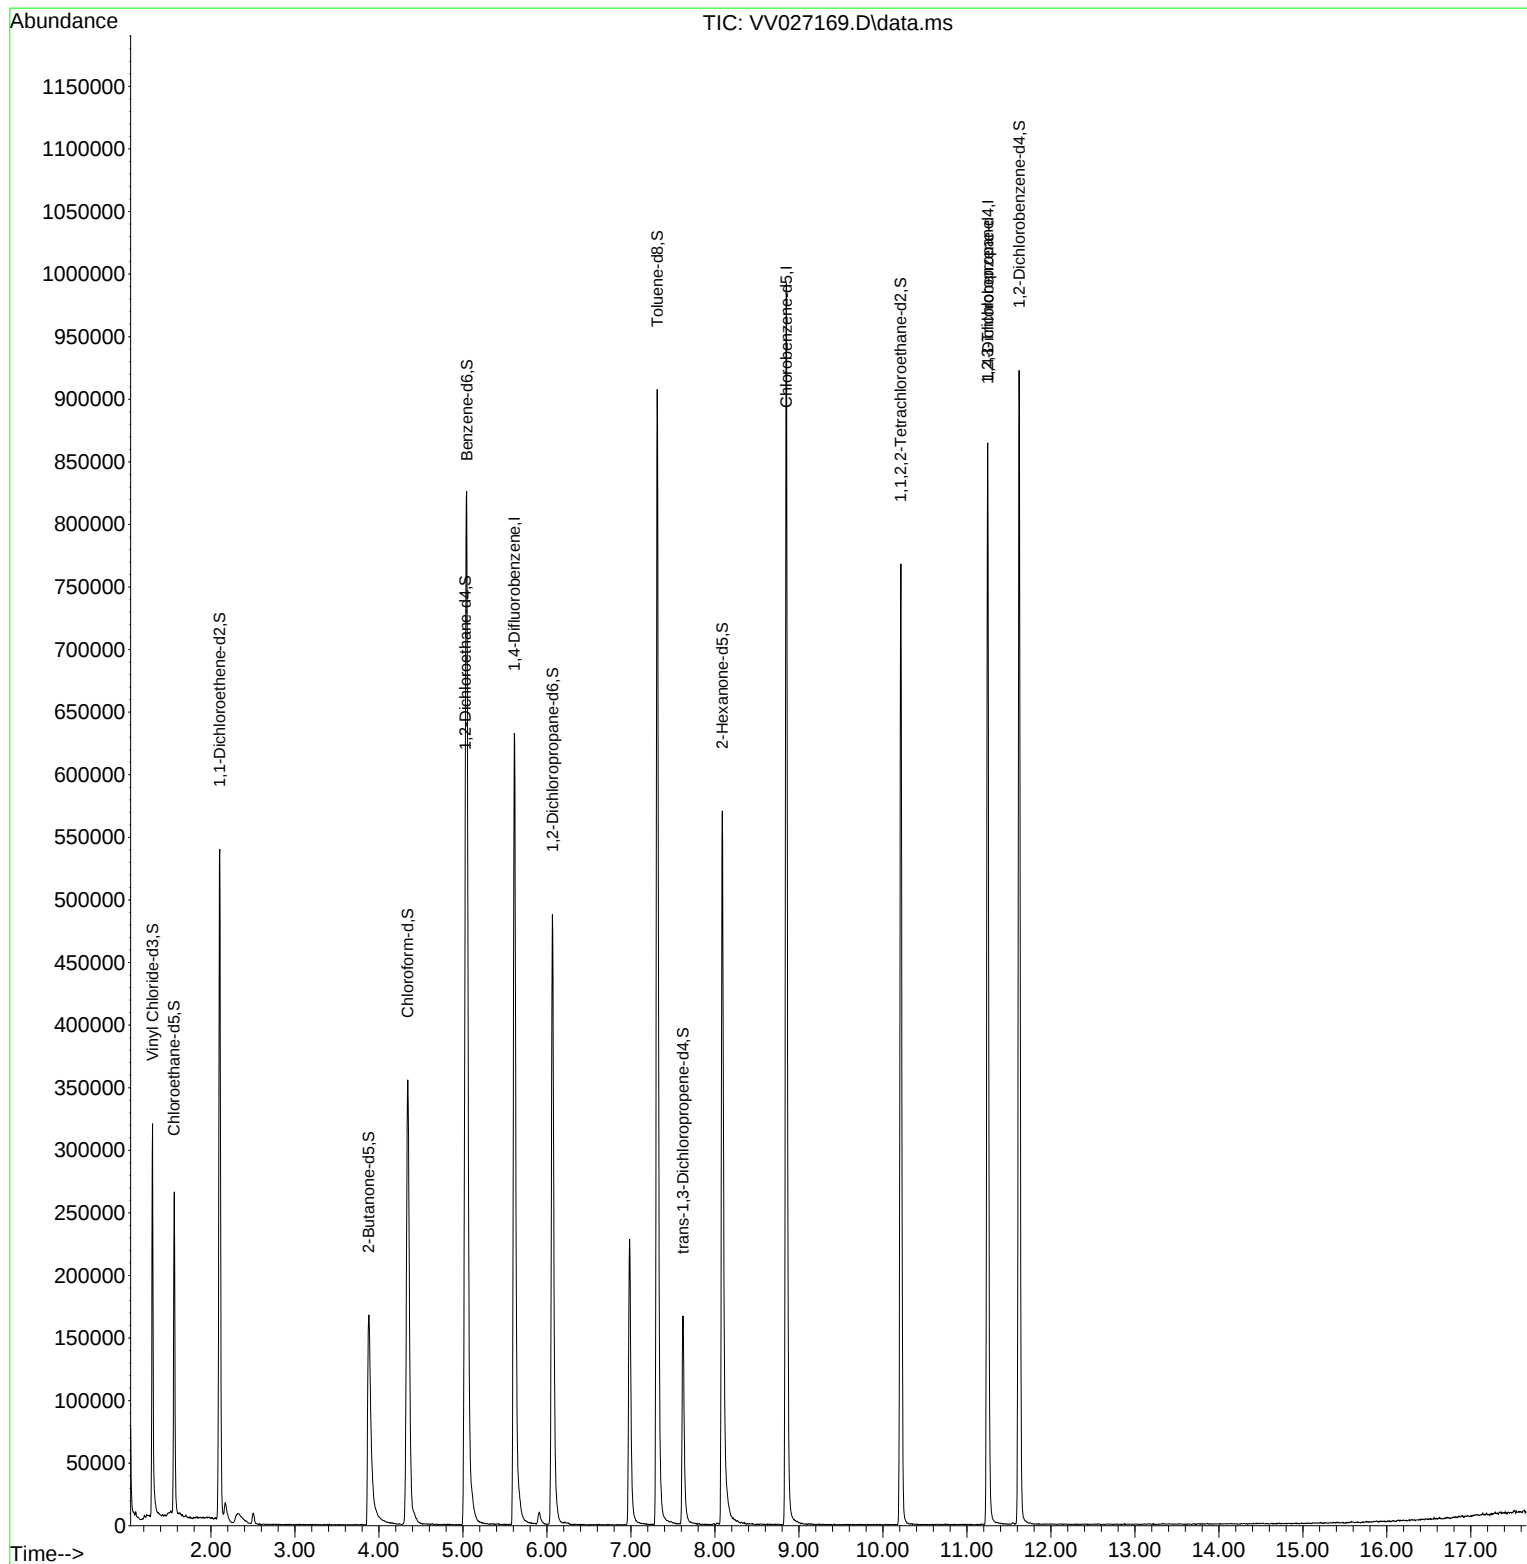

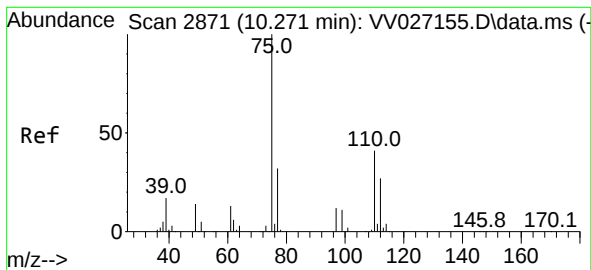

#61

1,2,3-Trichloropropane

Concen: 5.482 ug/L

RT: 11.246 min Scan# 31

Delta R.T. 0.974 min

Lab File: VV027169.D


Acq: 02 Aug 2022 13:49

Instrument :

MSVOA_V

ClientSampleId :

VHBLK001

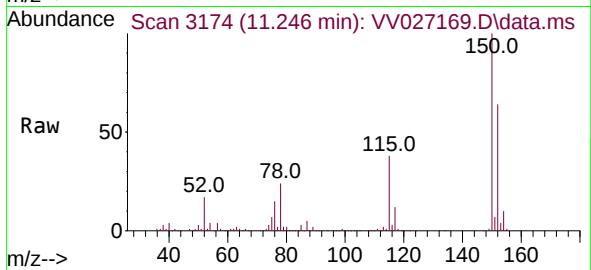

Tgt Ion: 75 Resp: 27261

Ion Ratio Lower Upper

75 100

77 30.8 25.8 38.8

110 2.6 32.8 49.2#

